

# Series 8000DH

CO<sub>2</sub> Incubator

Direct Heat with Sterilization Cycle

Operating and Maintenance Manual 7003540 Rev. 7



| Model | Sensor* | Voltage** |
|-------|---------|-----------|
| 3540  | T/C     | 115       |
| 3541  | T/C     | 230       |
| 3542  | IR      | 115       |
| 3543  | IR      | 230       |

\*T/C is a thermal conductivity sensor.

IR is an infra-red sensor.

\*\*All units are 50/60 Hz.

**MANUAL NUMBER 7003540**

| 7   | 25584         | 8/6/09   | Updated RH low alarm ringback time from 30 minutes to 15                      | ccs |
|-----|---------------|----------|---|-----|
| 6   | 25248/IN-3945 | 6/9/09   | Updated drawer specs - sliding and stationary                                 | ccs |
| 5   | 24900/IN-3923 | 4/22/09  | Updated door interlock switch (3598-200-9)                                    | ccs |
| 4   | 25303/IN-3902 | 2/17/09  | UL decom warning pg 1-6   | ccs |
| 3   | 24975         | 12/10/08 | Updated water specs on pages 1-10 and 1-11                                    | ccs |
| 2   | 24344/IN-3824 | 1/16/08  | Removed stud from back panel, chg'd grnd wire placement, updated CAD drawings | ccs |
| 1   | 24173         | 6/21/07  | Updated with Thermo data  | ccs |
| 0   | --            | 1/25/07  | Original manual   | ccs |
| REV | ECR/ECN       | DATE     | DESCRIPTION   | By  |



**Important** Read this instruction manual. Failure to read, understand and follow the instructions in this manual may result in damage to the unit, injury to operating personnel, and poor equipment performance. ▲

**Caution** All internal adjustments and maintenance must be performed by qualified service personnel. ▲

Material in this manual is for information purposes only. The contents and the product it describes are subject to change without notice. Thermo Fisher Scientific makes no representations or warranties with respect to this manual. In no event shall Thermo be held liable for any damages, direct or incidental, arising out of or related to the use of this manual.

**Warning** If the incubator is not used in the manner specified in this operating manual, the protection provided by the equipment design may be impaired. ▲

©2007 Thermo Fisher Scientific. All rights reserved.



Important operating and/or maintenance instructions. Read the accompanying text carefully.



Potential electrical hazards. Only qualified persons should perform procedures associated with this symbol.



Equipment being maintained or serviced must be turned off and locked off to prevent possible injury.



Hot surface(s) present which may cause burns to unprotected skin, or to materials which may be damaged by elevated temperatures.



Marking of electrical and electronic equipment, which applies to electrical and electronic equipment falling under the Directive 2002/96/EC (WEEE) and the equipment that has been put on the market after 13 August 2005.



This product is required to comply with the European Union's Waste Electrical & Electronic Equipment (WEEE) Directive 2002/96/EC. It is marked with the WEEE symbol. Thermo Fisher Scientific has contracted with one or more recycling/disposal companies in each EU Member State European Country, and this product should be disposed of or recycled through them. Further information on Thermo's compliance with this directive, the recyclers in your country and information on Thermo products will be available at [www.thermofisher.com](http://www.thermofisher.com).

- ✓ Always use the proper protective equipment (clothing, gloves, goggles, etc.)
- ✓ Always dissipate extreme cold or heat and wear protective clothing.
- ✓ Always follow good hygiene practices.
- ✓ Each individual is responsible for his or her own safety.

## Do You Need Information or Assistance on Thermo Scientific Products?

If you do, please contact us 8:00 a.m. to 6:00 p.m. (Eastern Time) at:

1-740-373-4763

Direct

1-800-438-4851

Toll Free, U.S. and Canada

1-740-373-4189

FAX

<http://www.thermo.com>

Internet Worldwide Web Home Page

[service.led.marietta@thermofisher.com](mailto:service.led.marietta@thermofisher.com)

Service E-Mail Address

Our **Sales Support** staff can provide information on pricing and give you quotations. We can take your order and provide delivery information on major equipment items or make arrangements to have your local sales representative contact you. Our products are listed on the Internet and we can be contacted through our Internet home page.

Our **Service Support** staff can supply technical information about proper setup, operation or troubleshooting of your equipment. We can fill your needs for spare or replacement parts or provide you with on-site service. We can also provide you with a quotation on our Extended Warranty for your Thermo Scientific products.

Whatever Thermo Scientific products you need or use, we will be happy to discuss your applications. If you are experiencing technical problems, working together, we will help you locate the problem and, chances are, correct it yourself...over the telephone without a service call.

When more extensive service is necessary, we will assist you with direct factory trained technicians or a qualified service organization for on-the-spot repair. If your service need is covered by the warranty, we will arrange for the unit to be repaired at our expense and to your satisfaction.

Regardless of your needs, our professional telephone technicians are available to assist you Monday through Friday from 8:00 a.m. to 6:00 p.m. Eastern Time. Please contact us by telephone or fax. If you wish to write, our mailing address is:

Thermo Scientific  
Controlled Environment Equipment  
401 Millcreek Road, Box 649  
Marietta, OH 45750

International customers, please contact your local Thermo Scientific distributor.

## Warranty Notes

### **Information You Should Know Before Requesting Warranty Service**

- **Locate the model and serial numbers.** A serial tag is located on the unit itself.
- For equipment service or maintenance, or with technical or special application inquiries, contact your local distributor.

### **Repairs NOT Covered Under Warranty**

- **Calibration of control parameters.** Nominal calibrations are performed at the factory; typically  $\pm 1^{\circ}\text{C}$  for temperature,  $\pm 1\%$  for gases, and  $\pm 5\%$  for humidity. Our service personnel can provide precise calibrations as a billable service at your location. Calibration after a warranty repair is covered under the warranty.
- **Damage resulting from use of improper quality water, chemicals or cleaning agents detrimental to equipment materials.**
- **Service calls for improper installation or operating instructions.** Corrections to any of the following are billable services:
  - 1) electrical service connection
  - 2) tubing connections
  - 3) gas regulators
  - 4) gas tanks
  - 5) unit leveling
  - 6) room ventilation
  - 7) adverse ambient temperature fluctuations
  - 8) any repair external to the unit
- **Damage resulting from accident, alteration, misuse, abuse, fire, flood, acts of God, or improper installation.**
- **Repairs to parts or systems resulting from unauthorized unit modifications.**
- **Any labor costs other than that specified during the parts and labor warranty period, which may include additional warranty on CO<sub>2</sub> sensors, blower motors, water jackets, etc.**



# Table of Contents

|                  |   |            |
|------------------|---|------------|
| <b>Section 1</b> | <b>Installation and Start-Up</b>                        | <b>1-1</b> |
|                  | Keypad Operation  | 1-3        |
|                  | Displays  | 1-4        |
|                  | Installing the Incubator                                | 1-4        |
|                  | Stacking the Incubators                                 | 1-5        |
|                  | Preliminary Cleaning                                    | 1-6        |
|                  | Shelf Installation                                      | 1-7        |
|                  | Access Port Filter & CO <sub>2</sub> Sensor Cover Plate | 1-8        |
|                  | Air Sample Filter Installation                          | 1-8        |
|                  | HEPA Filter Installation                                | 1-9        |
|                  | Leveling the Unit                                       | 1-9        |
|                  | Electrical Power Connection                             | 1-9        |
|                  | Filling the Humidity Pan                                | 1-10       |
|                  | Connecting the CO <sub>2</sub> Gas Supply               | 1-11       |
|                  | Incubator Start-Up                                      | 1-12       |
| <b>Section 2</b> | <b>Calibration</b>                                      | <b>2-1</b> |
|                  | Temperature   | 2-1        |
|                  | Thermal Conductivity CO <sub>2</sub> System             | 2-2        |
|                  | Infrared CO <sub>2</sub> System                         | 2-3        |
|                  | Relative Humidity                                       | 2-4        |




|                  |   |            |
|------------------|---|------------|
| <b>Section 3</b> | <b>Configuration</b> .....                                  | <b>3-1</b> |
|                  | Turn Audible Alarm ON/OFF .....                             | 3-1        |
|                  | New HEPA Filter .....                                       | 3-1        |
|                  | Set REPLACE HEPA filter reminder .....                      | 3-2        |
|                  | Set Access Code .....                                       | 3-2        |
|                  | Set Low Temp Alarm Limit (tracking alarm) .....             | 3-3        |
|                  | Enable Low Temp Alarm to Trip Contacts .....                | 3-3        |
|                  | Set Low CO <sub>2</sub> Alarm Limit (tracking alarm) .....  | 3-4        |
|                  | Set High CO <sub>2</sub> Alarm Limit (tracking alarm) ..... | 3-4        |
|                  | Enable CO <sub>2</sub> Alarms to Trip Contacts .....        | 3-5        |
|                  | Set New Zero Number for T/C CO <sub>2</sub> Sensors .....   | 3-5        |
|                  | Set New Span Number for T/C CO <sub>2</sub> Sensors .....   | 3-6        |
|                  | Setting a Low RH Alarm Limit .....                          | 3-6        |
|                  | Enable RH Alarms to Trip Contacts .....                     | 3-7        |
|                  | Enabling Temp/RH to be Displayed .....                      | 3-7        |
| <b>Section 4</b> | <b>Alarms</b> .....   | <b>4-1</b> |
|                  | Temp Controller Failure TMP CNTR ERR .....                  | 4-2        |
|                  | Sensor Fault Alarms .....                                   | 4-2        |
|                  | Preventive Maintenance .....                                | 4-3        |
| <b>Section 5</b> | <b>Routine Maintenance</b> .....                            | <b>5-1</b> |
|                  | Clean Cabinet Exterior .....                                | 5-2        |
|                  | Clean Glass Doors .....                                     | 5-3        |
|                  | Clean Humidity Pan .....                                    | 5-3        |
|                  | HEPA Filter Maintenance .....                               | 5-5        |
|                  | Replace Power Fuses .....                                   | 5-5        |
|                  | Replace Air Sample Filter .....                             | 5-6        |
|                  | Electronics Section .....                                   | 5-6        |
|                  | Sterilization Cycle .....                                   | 5-8        |

|                   |  |              |
|-------------------|--|--------------|
| <b>Section 6</b>  | <b>Factory Options</b> .....           | <b>.6-1</b>  |
|                   | Remote Alarms .....                    | .6-1         |
|                   | Humidity Readout .....                 | .6-2         |
| <b>Section 7</b>  | <b>Specifications</b> .....            | <b>.7-1</b>  |
| <b>Section 8</b>  | <b>Spare Parts</b> .....               | <b>.8-1</b>  |
|                   | Exploded Part Drawings .....           | .8-2         |
| <b>Section 9</b>  | <b>Electrical Schematics</b> .....     | <b>.9-1</b>  |
| <b>Section 10</b> | <b>Warranty Information</b> .....      | <b>.10-1</b> |
| <b>Section 11</b> | <b>Declaration of Conformity</b> ..... | <b>.11-1</b> |



# Section 1 Installation and Start-Up

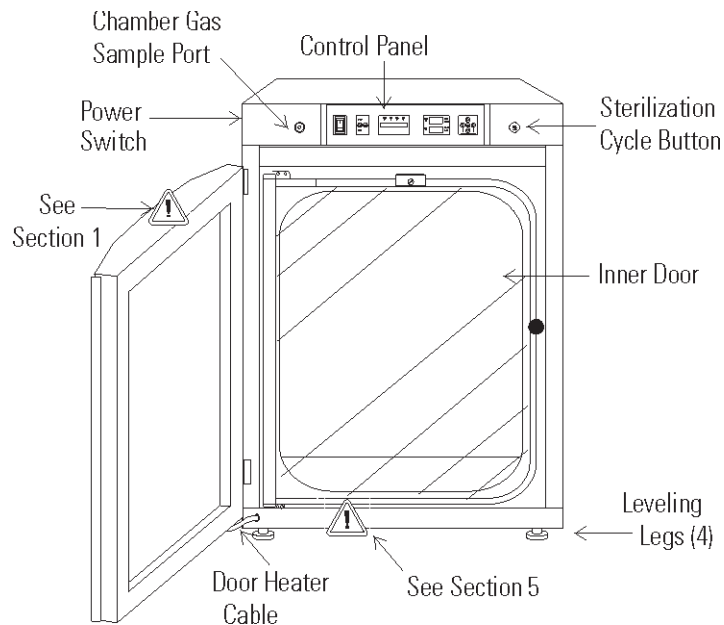


**Figure 1-1.** Components

- Chamber Gas Sample Port - Used for sampling chamber CO<sub>2</sub> content using a FYRITE or similar instrument.
- Main Power Switch - Mains Disconnect
- Control Panel - Keypad, displays & indicators (Figure 1-2)
- Leveling Legs - Used to level the unit
- Sterilization Cycle Button - Switch to initiate sterilization cycle

**Note** The incubators are stackable. Information follows. ▲

- ☐ - Mutes the audible alarm.
- Alarm Indicator - Light pulses on/off during an alarm condition.
- MODE** Select Switch - Used to select Run, Setpoints, Calibration and Configuration modes.
- Message Display - Shows system status.
- Mode Select Indicators -
  - RUN: Run Menu
  - SET: Set Points Menu
  - CAL: Calibration Menu
  - CON: Configuration Menu
- HEAT** Indicator - Lights when heaters are activated.
- INJ** Indicator - Lights during CO<sub>2</sub> injection into chamber.
- T (°C) Display - Programmable to display temperature. See Configuration section.
- RH (%) Display - Shows percentage of humidity. See Configuration section.
- CO<sub>2</sub> (%) Display - Programmable to display CO<sub>2</sub> percentage. See Configuration section.
- Arrow Keys (Scroll for Parameters) - Increases or decreases number values, toggles between mode choices.
- ENTER** - Stores the selected value into unit memory.

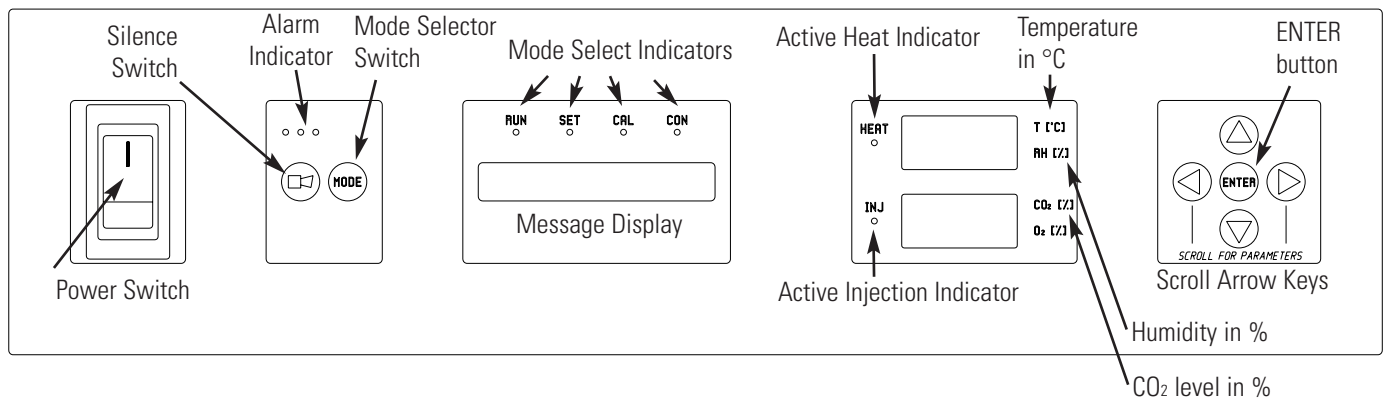

**Figure 1-2.** Control Panel

# Keypad Operation

The Series 8000DH incubator has four basic modes for incubator setup: Run, Setpoints, Calibration and Configuration.

- Run is the default mode for normal operation.
- Set is used to enter system setpoints for incubator operation.
- Calibration is used to calibrate various system parameters.
- Configuration allows for custom setup of various options.

**Table 1-1.** Selections Under Each Mode

| RUN          | SETPOINT                                   | CALIBRATION   | CONFIGURATION   |
|--------------|--|---|---|
| Default Mode | Temperature<br>Overtemp<br>CO <sub>2</sub> | Temp Offset<br>CO <sub>2</sub> Cal <sup>1</sup><br>IR Cal <sup>2</sup><br><i>RH Cal</i> | Audible<br>New HEPA Timer<br>Replace HEPA Reminder<br>Access Code<br>Temp Lo Alarm<br>Temp Relay<br>CO <sub>2</sub> Lo Alarm<br>CO <sub>2</sub> Hi Alarm<br>CO <sub>2</sub> Relay<br>CO <sub>2</sub> Z & S #'s *<br><i>RH Lo Alarm</i><br><i>RH Relay</i><br><i>Display Temp</i><br><i>Display RH</i> |
|              |  | <b>Base Unit Displays</b><br><i>Option Unit Displays</i>                                |   |


<sup>1</sup> T/C units  
<sup>2</sup> IR units  
\*T/C units only

## Keypad Operation (continued)

**SCROLL FOR PARAMETERS Arrows:** Steps the operator through parameters of SET, CAL and CON modes. The right arrow goes to the next parameter, the left arrow returns to the previous parameter.

**Up/Down Arrows:** Increases/decreases or toggles the parameter value selected in SET, CAL, and CON modes.

**ENTER:** Must press this key to save-to-memory all changed values.

 **Key:** Press to mute audible alarm. See Section 4 for alarm ringback times.

## Displays

**Message Display:** Shows system status (Mode) at all times. Shows 'CLASS 100' or 'SYSTEM OK' during normal operation, or alarm messages if the system detects an alarm condition (see Section 4, Alarms). The message 'CLASS 100' is a timing mechanism indicating that, under normal operating conditions with the HEPA filter installed, the air inside the chamber meets the Class 100 air cleanliness standard for particulates of 0.5 micron size or larger per cubic foot of air. Further information on the Class 100 classification of air quality is available from Thermo.

**Upper and Lower Displays:** The 7 segment upper display shows temp and RH. The lower display shows CO<sub>2</sub> and O<sub>2</sub>.

## Installing the Incubator


1. Maintain a minimum three inch clearance behind the incubator for electrical and gas hook-ups. In addition, a three inch ventilation space is needed on each side.
2. Locate the unit on a firm level surface capable of supporting the unit weight of 260 lbs (118kg).
3. Locate the unit away from doors and windows and heating and air conditioning ducts.
4. Lift the unit by the sides of the cabinet base. Do not attempt to lift it by the front and back. This places stress on the outer door hinges.

## Stacking the Incubators

**Warning** Install stacked units against a wall or similar structure. ▲

**Warning** With incubators in a stacked configuration, do not leave both exterior doors open at the same time. ▲


**Warning** If the units have been in operation, turn them both off and disconnect the power source before beginning any service work. ▲




Two stacking brackets (shown at left) are included in the parts bag shipped with each incubator.

**Figure 1-3.** Stacking Brackets

1. Remove the cover plate securing the door cord from the incubator to be on top. See Figure 1-4. Disconnect the plug from the connector.
2. Remove the four screws securing the door hinges to the unit. Remove the door and set it aside.

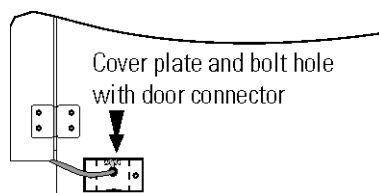


**Figure 1-4.** Cover Plate

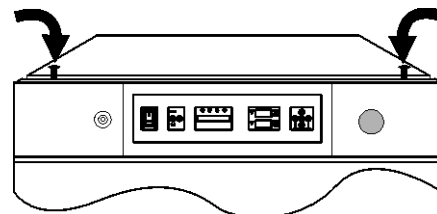

**Figure 1-5.** Hole Plug Locations

3. Unscrew the two hole plugs from the top cover of the incubator to be the bottom of the stack (Figure 1-5).
4. Unscrew and remove the 4 leveling feet from the unit to be stacked on top and lift it onto the bottom unit. Align all sides.

**Warning** This incubator weighs 260 lbs (118kg). Have sufficient personnel available when lifting. Lift the unit by the sides of the cabinet base to avoid placing stress on the outer door hinge. ▲

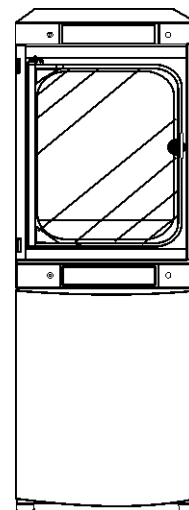


**Figure 1-6.** Bolt Holes




## Stacking the Incubators (cont.)

5. Insert the stacking brackets into the slots at the back of the stacked units as shown in Figure 1-7.
6. Align the slotted holes in the brackets with the mounting holes on the back of the top incubator. Secure the brackets with the screws and washers provided in the parts bag. See Figure 1-8.

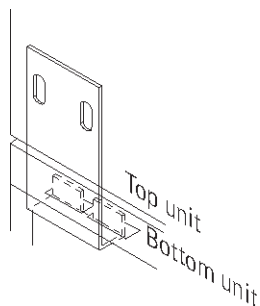


**Figure 1-7.** Bracket into Slot

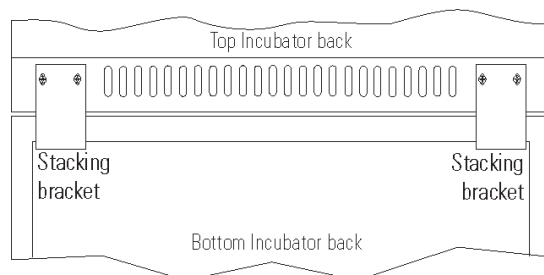

**Figure 1-8.** Installed Brackets on Back of Unit

7. Thread one 1/4 x 20 bolt and washer included with the stacking brackets, into the hole behind the cover plate. Do not tighten. Refer to Figure 1-9.
8. Remove the cover plate from the same area on the other side of the top unit.
9. Thread the other 1/4 x 20 bolt and washer into this hole.

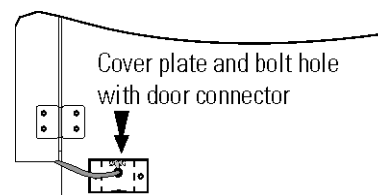

**Figure 1-9.** Bolt Hole

10. Tighten the bolts on both sides.
11. Assemble the door hinges to the unit. Secure with the screws.
12. Plug the door cord into the connector, as previously. Secure the cover plate.
13. Install the cover plate on the other side of the unit. The stacked incubators are ready for service.



## Preliminary Cleaning

1. Remove vinyl from shelf channels, duct sheets, and air duct, if present.
2. Using a suitable laboratory disinfectant, clean all interior surfaces.

**Caution** Before using any cleaning or decontamination method except those recommended by the manufacturer, users should check with the manufacturer that the proposed method will not damage the equipment. Accidental spills of hazardous materials on or inside this unit are the responsibility of the user. ▲

## Shelf Installation

1. Install the large sheet metal side ducts with the tabs facing into the center of the chamber with their slots up. There are no right side or left side ducts, simply rotate one of them to fit the opposite side. Tilt the side ducts as they are placed into the chamber so the tops fit into the top air duct, then guide them into the vertical position. Figure 1-10 shows the side duct as it would be oriented for the right side of the chamber.

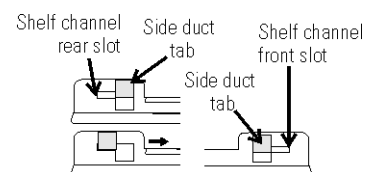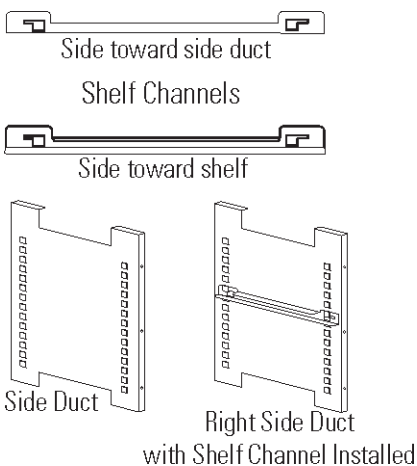


**Figure 1-10.** Shelf Channels and Side Ducts      **Figure 1-11.** Channels and Slots

2. Referring to Figure 1-10, note that there is no difference in the left and right shelf channels.
3. Install the shelf channels by placing the channel's rear slot over the appropriate rear tab on the side duct. Pull the shelf channel forward and engage the channel's front slot into the side duct's appropriate forward tab. Refer to Figure 1-11.
4. Figure 1-10 shows one of the channels installed on the right side duct.

## Access Port Filter & CO<sub>2</sub> Sensor Cover Plate


1. Locate the opening in the top left corner of the interior chamber. Remove the tape from the opening on the outside of the unit.
2. Locate the stopper with filter in the hardware bag. Lift the metal port cover and install the assembly in the opening inside the chamber. See Figure 1-12.
3. Also in the hardware bag is the CO<sub>2</sub> sensor cover plate. Install, using the 1/4-turn fasteners. Refer to Figure 1-12 for the location.

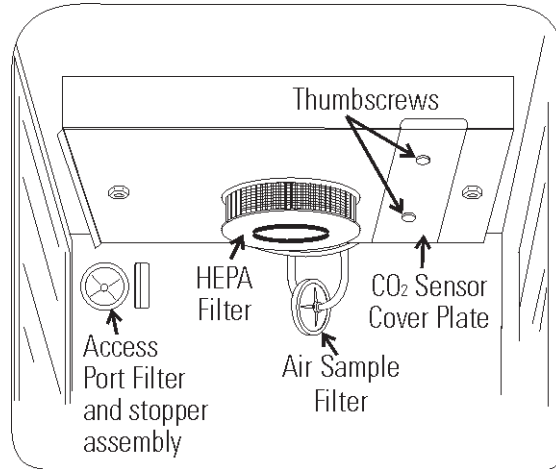

**Figure 1-12.** Filter and Plate

## Air Sample Filter Installation

1. Remove the filter from the shipping bag.
2. Install the air sample filter assembly to the black hose barb behind the top duct.
3. Insert the other end of the filter assembly onto the metal tubing on the top duct. Refer to the Figure 1-13.

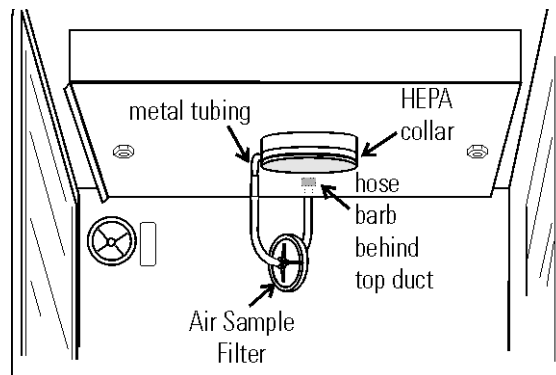

**Figure 1-13.** Air Sample Filter Installation

## HEPA Filter Installation

**Caution** Be careful when the filter. The media can be damaged if it is mishandled. To avoid damage to the incubator, do not operate the unit without the HEPA filter in place. ▲

1. Remove the filter from the shipping box.
2. Remove the plastic coating from the filter, using caution not to touch the filter media.
3. Install the filter as shown in Figure 1-13. Refer to Section 5 for HEPA filter maintenance.

**Caution** The media of the filter can be damaged if mishandled. To avoid damage to the incubator, do not operate the unit without the HEPA filter in place. ▲

## Leveling the Unit

Check the unit for being level by placing a bubble-style level on one of the shelves. Turn the hex nut on the leveler counterclockwise to lengthen the leg or clockwise to shorten it. Level the unit front-to-back and left-to-right.

## Electrical Power Connection


See the serial tag on the side of the unit for electrical specifications or refer to the electrical schematics at the end of this manual.

**Caution** Serial tag rating is based on amperage draw during sterilization cycle. Normal operating amperage is much less. Ensure that electrical circuit will handle amp draw of sterilization cycle.

Connect the incubator to a grounded, dedicated circuit. The power cord connector is the mains disconnect device for the incubator. Position the unit so that it can be easily disconnected. ▲

## Electrical Power Connection (cont.)

Plug the provided power cord into the power inlet connector on the back of the cabinet (Figure 1-14), then into the grounded, dedicated, electrical circuit.

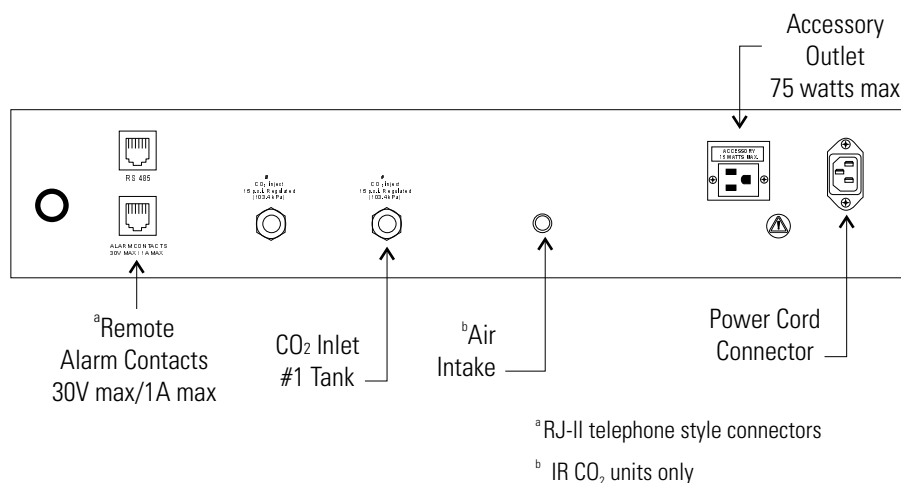

**Figure 1-14.** Back of Cabinet

## Filling the Humidity Pan

Fill the humidity pan with sterile distilled water to within 1/2” of the top. Place the pan directly in the center of the incubator floor.

For applications requiring high humidity, the pan should be placed against the left side wall of the incubator. The side ducts have been modified to allow the pan to be placed against the wall. Optimum humidity is achieved by capping the CO<sub>2</sub> sample port. This will, however, cause condensation in the chamber. To enhance RH recovery from door openings, place a second humidity pan in the right side duct.

For best operation of the incubator, sterilized distilled, demineralized or de-ionized water should be used in the humidity pan. Water purity should be in the resistance range of 50K to 1M Ohm/cm, or a conductivity range of 20.0 to 1.0 uS/cm. Refer to ASTM Standard D5391-93 or D4195-88 for measuring water purity.

Distillation systems, as well as some types of reverse osmosis water purity systems, can produce water in the quality range specified. Tap water is not recommended as it may contain chlorine, which can deteriorate the stainless steel. Tap water may also have a high mineral content, which would produce a build-up of scale in the pan. High purity or ultra pure water is not recommended as it is an extremely aggressive solvent and will deteriorate the stainless steel.

## Filling the Humidity Pan (continued)

High purity water has a resistance of above 1M to 18M Ohm. Even high purity water can contain bacteria and organic contaminants. Water should always be sterilized or treated with a decontaminant, safe for use with stainless steel as well as safe for the product, prior to being introduced into the humidity pan.

Check the level and change the water frequently to avoid contamination. Do not allow the water level to fluctuate significantly. “Dry-outs” will have an adverse effect on the humidity level and CO<sub>2</sub> calibration of the T/C units.

**Caution** Use of chlorinated water, or decontamination products containing chlorine, will deteriorate the stainless steel and cause rust, voiding the warranty. ▲

## Connecting the CO<sub>2</sub> Gas Supply

**Warning** High concentrations of CO<sub>2</sub> gas can cause asphyxiation! OSHA Standards specify that employee exposure to carbon dioxide in any eight-hour shift of a 40-hour work week shall not exceed the eight-hour time weighted average of 5000 PPM (0.5% CO<sub>2</sub>). The short term exposure limit for 15 minutes or less is 30,000 ppm (3% CO<sub>2</sub>). Carbon dioxide monitors are recommended for confined areas where concentrations of carbon dioxide gas can accumulate. ▲

**Warning** This incubator is designed to be operated with CO<sub>2</sub> gas only. Connecting a flammable or toxic gas can result in a hazardous condition. Gases other than CO<sub>2</sub> should not be connected to this equipment. CO<sub>2</sub> gas cylinders have a UN1013 label on the cylinder and are equipped with a CGA 320 outlet valve. Check the gas cylinder for the proper identification labels. The CO<sub>2</sub> gas supply being connected to the incubator should be industrial grade, 99.5% pure. Do not use CO<sub>2</sub> gas cylinders equipped with siphon tubes. A siphon tube is used to extract liquid CO<sub>2</sub> from the cylinder which can damage the pressure regulator. Consult with your gas supplier to ensure that the CO<sub>2</sub> cylinder does not contain a siphon tube. Gas cylinders should also be secured to a wall or other stationary object to prevent them from tipping.

A two-stage CO<sub>2</sub> pressure regulator is required to be installed on the outlet valve of the gas cylinder. Input pressure to the incubator must be maintained at 15 psig (103.4 kPa) for proper performance of the CO<sub>2</sub> control system. A single stage CO<sub>2</sub> pressure regulator will not maintain 15 psig (103.4 kPa) to the incubator as the pressure in the CO<sub>2</sub> cylinder decreases; therefore, a two stage regulator is recommended.

## Connecting CO<sub>2</sub> Gas Supply (continued)

**Warning** If higher purity CO<sub>2</sub> is desired inside the incubator (greater than 99.5% pure), the pressure regulator should be constructed with a stainless steel diaphragm, along with specifying the purity of the CO<sub>2</sub> from the gas supplier. Follow the manufacturer's instructions to ensure proper and safe installation of the pressure regulator on the gas cylinder.

Consult your facility safety officer to ensure that the equipment is installed in accordance with the codes and regulations that are applicable in your area. ▲

The CO<sub>2</sub> gas supply being connected should be industrial grade 99.5% pure and should not contain siphon tubes. Install a two-stage pressure regulator at the cylinder outlet. The high pressure gauge at the tank should have 0-2000 psig range. The low pressure gauge, at the incubator inlet, should have a 0-30 psig range. Input pressure to the incubator must be maintained at 15 psig (103.4 kPa).

The incubator has serrated fittings on the back of the cabinet to connect the gas supply. Refer to Figure 1-14. The fitting is labeled CO<sub>2</sub> Inlet #1 Tank. Make sure that the connections are secured with clamps. Check all fittings for leaks.

## Incubator Start-Up

With the incubator properly installed and connected to power, the humidity pan filled, and the unit connected to gas supplies, system setpoints can be entered. The following setpoints can be entered in SET mode: Temperature, Overtemperature and CO<sub>2</sub>. To enter SET mode, press the MODE key until the SET indicator lights. Press the right and/or left arrow keys until the proper parameter appears in the message display. See Chart 1-1 for more detail.

## Setting the Operating Temperature

All Series 8000DH incubators have an operating temperature range of 10°C to 50°C, depending on ambient temperature. The incubator is shipped from the factory with a temperature setpoint of 10°C. At this setting, all heaters are turned off.

## Setting the Operating Temperature (continued)

To change the operating temperature setpoint:

1. Press the MODE key until the SET indicator lights.
2. Press the right arrow until “Temp XX.X” is displayed in the message display.
3. Press the up/down arrow key until the desired temperature setpoint is displayed.
4. Press ENTER to save the setpoint.
5. Press the MODE key until the RUN indicator lights for RUN mode or press the right/left arrow keys to go to next/previous parameter.

## Setting the Overtemp Setpoint

**Caution** The independent overtemp system is designed as a safety to protect the incubator only. It is not intended to protect or limit the maximum temperature of the cell cultures or customer’s equipment inside the incubator if an overtemp condition occurs. ▲

Series 8000DH incubators are equipped with a secondary temperature monitoring system to monitor the air temperature inside the cabinet. This system is designed as a safety device to turn off all heaters in the event of a temperature control failure. Temperature control in the incubator will be  $\pm 1^\circ$  of the overtemp setpoint.

The overtemperature is set by the factory (default) at 40°C. However, the overtemp can be set up to 55°C in 0.5° increments.

If the incubator’s operating temperature setpoint is set above the overtemp setpoint, the overtemp setpoint will automatically update to 1°C above the temperature setpoint. It is recommended that the overtemp setpoint be maintained at 1°C over the operating temperature setpoint.



## Setting the Overtemp Setpoint (continued)

To set the Overtemp setpoint:

1. Press the MODE key until the SET indicator lights
2. Press the right arrow until Otemp XX.X is displayed in the message display
3. Press the up or down arrow key until the desired Overtemp setpoint is displayed
4. Press ENTER to save the setting
5. Press the MODE key until the RUN indicator lights or press the right or left arrow to go to the next or previous parameter.


## Setting the CO<sub>2</sub> Setpoint

All T/C CO<sub>2</sub> cells are calibrated at the factory at 37°C, high humidity, and 10% CO<sub>2</sub>. Therefore, if a temperature setpoint of 37°C has been entered, the humidity pan has been filled and the CO<sub>2</sub> control is to run between 0-10% with a T/C CO<sub>2</sub> sensor, the CO<sub>2</sub> setpoint may be entered immediately. Otherwise, it is important to allow the unit 12 hours to stabilize at the temperature setpoint before entering the CO<sub>2</sub> setpoint.

Both models of the incubator have a CO<sub>2</sub> setpoint range of 0.0% to 20.0%. The incubator is shipped from the factory with a CO<sub>2</sub> setpoint of 0.0%. At this setting, all CO<sub>2</sub> control and alarms are turned off. To change the CO<sub>2</sub> setpoint:

1. Press the MODE key until the SET indicator lights.
2. Press the right arrow until "CO<sub>2</sub> XX.X" is displayed in the message display.
3. Press the up/down arrows until the desired CO<sub>2</sub> setpoint is displayed.
4. Press ENTER to save the setpoint.
5. Press the MODE key until the RUN indicator lights to go to RUN mode or press the right/left arrow keys to go to next/previous parameter.

# Chart 1-1. Set Mode

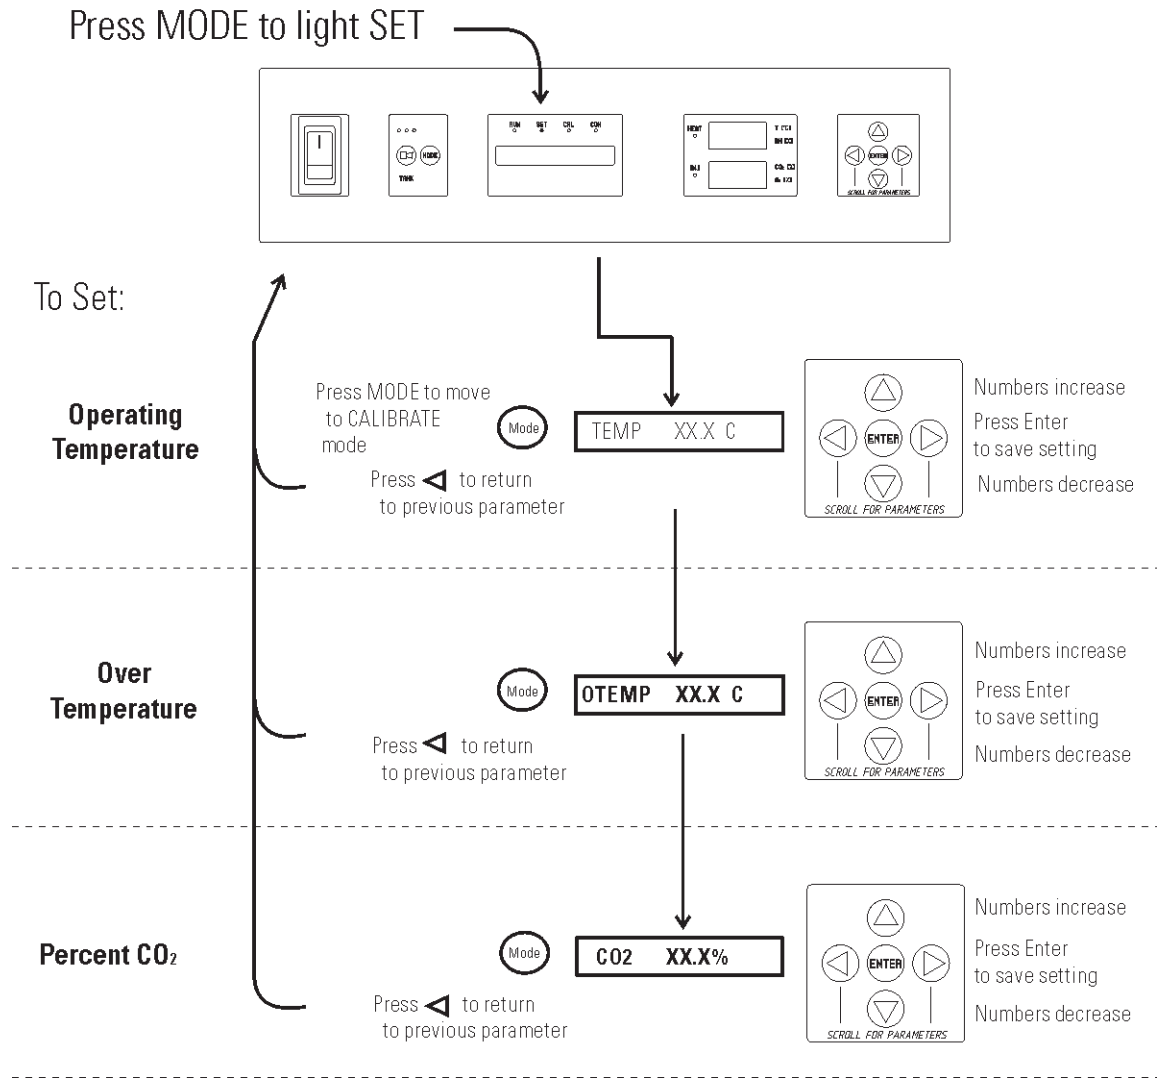



## Section 2 Calibration

After the unit has stabilized, several different systems can be calibrated. In Calibration mode, the air temperature, CO<sub>2</sub> and RH levels can be calibrated to reference instruments. To access Calibration mode, press the MODE key until the CAL indicator lights. Press the right and/or left arrow until the appropriate parameter appears in the message display. See Chart 2-1 at the end of this section for more detail.

Calibration frequency is dependent on use, ambient conditions and accuracy required. A good laboratory practice would require at least an annual calibration check. On new installations, all parameters should be checked after the stabilization period.

Prior to calibration, the user should be aware of the following system functions. While the unit is in Calibration mode, all system control functions are stopped so the unit remains stable. Readout of the system being calibrated appears on the message display. If no keys are pressed for approximately five minutes while in Calibration mode, the system resets to RUN mode so control functions are reactivated.

**Caution** Before making any calibration or adjustments to the unit, it is imperative that all reference instruments be properly calibrated. ▲

### Temperature

Before calibration, allow the cabinet temperature to stabilize. Place the calibrated instrument in the center of the chamber. The instrument should be in the airflow, not against the shelf.

#### Temperature Stabilization Periods

Startup - Allow 12 hours for the temperature in the cabinet to stabilize before proceeding.

Already Operating - Allow at least 2 hours after the display reaches setpoint for temperature to stabilize before proceeding.

## Temperature (continued)

1. Press the MODE key until CAL indicator lights.
2. Press the right arrow until “TEMPCAL XX.X” appears in the message display.
3. Press up/down arrow to match display to calibrated instrument.
4. Press ENTER to store calibration.
5. Press the MODE key to return to RUN or the right/left arrow to go to next/previous parameter.

## Thermal Conductivity CO<sub>2</sub> System

Models 3540 and 3541 have a thermal conductivity (T/C) CO<sub>2</sub> sensor. Thermal conductivity of the incubator atmosphere is not only effected by the quantity of CO<sub>2</sub> present but also by the air temperature and water vapor present in the incubator atmosphere. In monitoring the effects of CO<sub>2</sub>, air temperature and absolute humidity must be held constant so any change in thermal conductivity is caused by a change in CO<sub>2</sub> concentration.

Changing temperature or changing from elevated humidity to room ambient humidity levels will necessitate a re-calibration of the CO<sub>2</sub> control.

Some T/C CO<sub>2</sub> sensors go through an aging period, especially on new installations. Calibration should be checked on a weekly basis, and adjusted as necessary. When stabilization occurs, checks can become less frequent.

### T/C CO<sub>2</sub> Sensor Stabilization Periods

**Start -Up** - The CO<sub>2</sub> sensor has been calibrated at the factory for 37°C and elevated humidity. Allow the temperature, humidity, and CO<sub>2</sub> levels in the chamber to stabilize at least 12 hours before checking the CO<sub>2</sub> concentration with an independent instrument.

**Presently Operating** - Make sure the chamber doors are closed. Allow at least 2 hours after the temperature and CO<sub>2</sub> displays reach their setpoints for chamber atmosphere stabilization.

## **Thermal Conductivity CO<sub>2</sub> System (continued)**

1. Make sure the stabilization periods outlined above are followed.
2. Sample the chamber atmosphere through the sample port with an independent instrument. Sample the atmosphere at least 3 times to ensure accuracy of the instrument.
3. Press the MODE key until the CAL indicator lights.
4. Press the right arrow until “CO<sub>2</sub> CAL XX.X” is displayed in the message display.
5. Press the up /down arrows to change the display to match the independent instrument.
6. Press ENTER to store the calibration.
7. Press the MODE key to return to RUN or the right or left arrows to go to the next/ previous parameter.

## **Infrared CO<sub>2</sub> System**

Models 3542 and 3543 have an infrared (IR) CO<sub>2</sub> sensor. Infrared CO<sub>2</sub> sensors are not effected by chamber atmosphere temperature or humidity. However, the light detector in the sensor is effected by wide temperature changes. Therefore, changing temperature setpoints could necessitate a recalibration of the CO<sub>2</sub>. Chamber temperature should be allowed to stabilize before checking CO<sub>2</sub> concentrations with an independent instrument, especially on start-up.

### **IR CO<sub>2</sub> Sensor Stabilization Times**

**Start-Up-** Allow the temperature and the CO<sub>2</sub> of the cabinet to stabilize at least 12 hours before proceeding.

**Presently Operating** - Allow CO<sub>2</sub> to stabilize at least 2 hours at setpoint before proceeding.

## Infrared CO<sub>2</sub> System (continued)

1. Measure the CO<sub>2</sub> concentration in the chamber through the gas sample port with a Fyrite or other independent instrument. Several readings should be taken to ensure accuracy.
2. Press the MODE key until the CAL indicator lights.
3. Press the right arrow until “IR CAL XX.X” appears in the message display.
4. Press the up/down arrow to adjust the display to match the independent instrument reading.
5. Press ENTER to store the calibration.
6. Press the MODE key to return to RUN mode.

## Relative Humidity

Model 3540 and 3541 incubators are equipped with an optional direct-readout relative humidity sensor. This is a readout only of the chamber relative humidity level. It does not provide any control of the relative humidity in the cabinet.

### Relative Humidity Stabilization Times

**Start-Up** - Allow 12 hours for the relative humidity and temperature in the chamber to stabilize before proceeding.

**Already Operating** - Allow at least 2 hours after temperature display reaches setpoint for relative humidity to stabilize before proceeding.

1. Place an accurate independent instrument in the center of the chamber. Allow at least 30 minutes for RH to stabilize.
2. Press the MODE key until the CAL indicator lights.
3. Press the right arrow key until “RH CAL XX” appears in the message display.
4. Press the up/down arrow to match the display to the independent instrument.
5. Press ENTER to store the calibration.
6. Press the MODE key to return to RUN mode.

## **Relative Humidity (continued)**


If a reliable RH measuring device is not available, the display can be calibrated to a typical level;

1. Follow the RH stabilization periods outlined above.
2. With a full humidity pan and stable temperature, the relative humidity in the chamber will be 95%.
3. Using Step 3-5 of the relative humidity sensor adjustment, adjust the display to 95%.

This calibration method should be accurate to within 5%.



# Chart 2-1. Calibration Mode

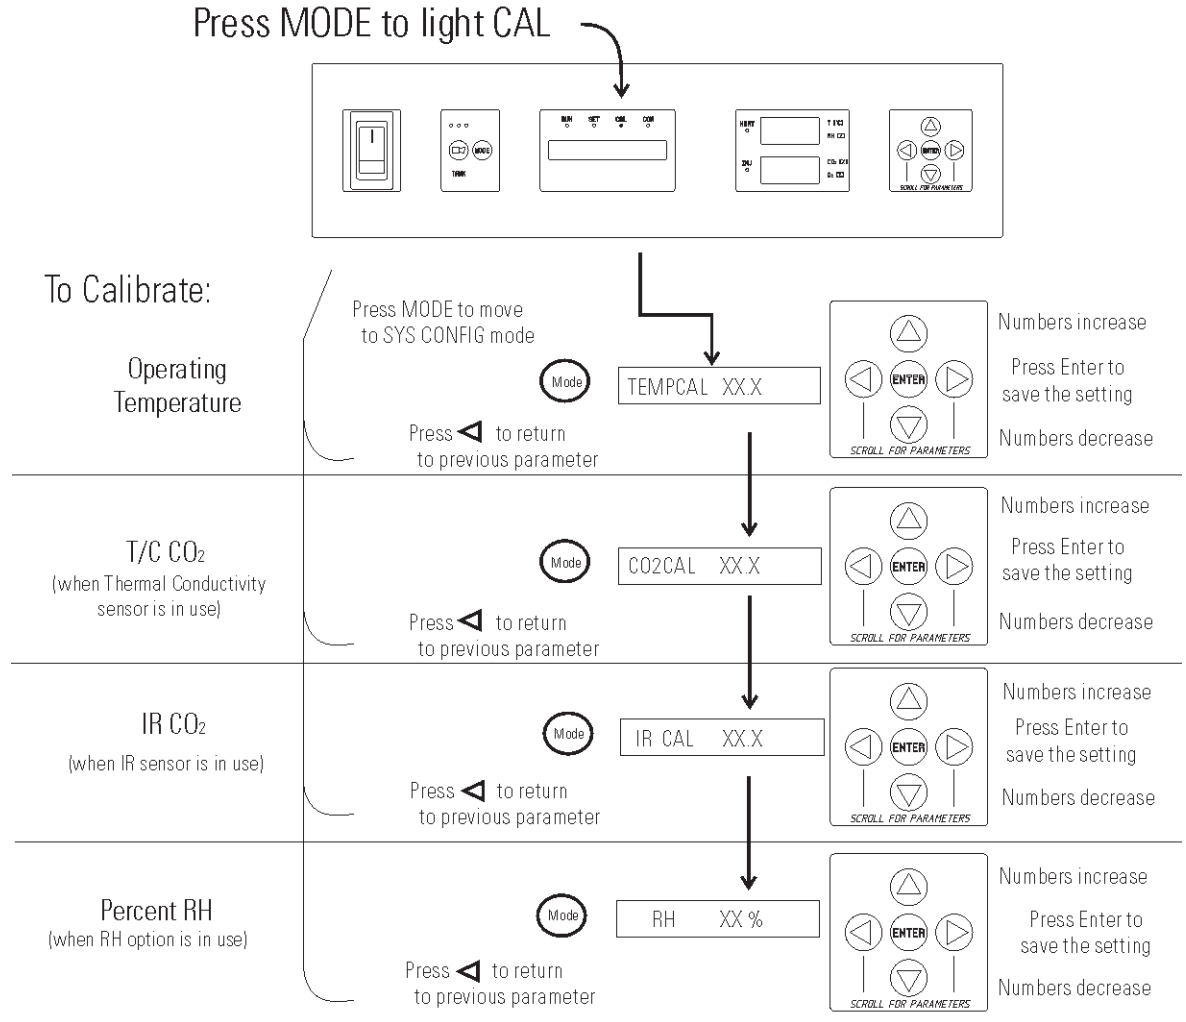

## Section 3 Configuration

Several features available in Configuration mode allow custom setup of the incubator. These features are listed with descriptions below. All features may not be necessary in all applications, but are available if needed. To enter Configuration mode, press the MODE key until the CON indicator lights. Press the right and/or left arrow until the appropriate parameter appears in the message display. See Chart 3-1 for more detail.

### Turn Audible Alarm ON/OFF

The audible alarm can be turned on or off. The factory setting is ON.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until AUDIBLE XXX shows in the message display.
3. Press the up/down arrow to toggle AUDIBLE ON/OFF.
4. Press ENTER to save the setting.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

### New HEPA Filter

When the REPLACE HEPA reminder displays and the visual alarm flashes, the specified time has elapsed and the HEPA filter should be replaced. To clear the display and reset the timer after replacing the HEPA filter with a new one, follow the steps below.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until NEW HEPA shows in the message display.
3. Press ENTER to restart the timer and clear the REPLACE HEPA alarm.
4. Press the MODE key to return to RUN mode.

## Set REPLACE HEPA filter reminder

A HEPA filter replacement timer can be set for a specific amount of time, from 1 to 12 months of actual unit running time. Time will not accrue when the unit is turned off. The default time is 6 months. When the allotted time runs out, REPLACE HEPA appears in the display and the visual alarm flashes. To set the reminder, use the following procedure.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until REPL HEPA XX is displayed.
3. Press the up/down arrow to choose the number of months desired.
4. Press ENTER to save the number.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

**Note** After the reminder has been set, check the allotted time remaining by going to Configuration mode, then pressing the right arrow until NEW HEPA XXX displays. This number is the remaining days before the filter replacement time specified runs out. For example, if 12 months was chosen in the REPL HEPA XX message display, the NEW HEPA number would be 365 days. ▲

## Set Access Code

A 3-digit Access Code can be entered to avoid unauthorized personnel from changing the setpoints, calibration, or configuration. A setting of 000 bypasses the access code. The factory setting is 000.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until ACC CODE XXX shows in the message display.
3. Press up/down arrow to change the access code.
4. Press ENTER to save the access code.
5. Press the MODE key to return to the RUN mode or right/left arrow to go to next/previous parameter.

## **Set Low Temp Alarm Limit (tracking alarm)**

The low temp alarm limit is the deviation from the temperature setpoint which causes a low temp alarm. The low temp alarm is variable from 0.5° below setpoint to 5° below setpoint. The factory setting is 1° below setpoint. A minus sign (-) in the display indicates that the alarm setting is below the setpoint.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until TEMP LO -X.X shows in the message display.
3. Press up/down arrow to change the low temp alarm limit.
4. Press ENTER to save the low temp alarm limit.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

## **Enable Low Temp Alarm to Trip Contacts**

The low temperature alarm can be programmed to trip the remote alarm contacts. A setting of ON allows this, an OFF setting blocks the low temp alarm from tripping the contacts. The factory setting is ON.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until TMP RLY XXX displays.
3. Press the up/down key to toggle the setting ON/OFF.
4. Press ENTER to save the setting
5. Press the MODE key to return to RUN mode, or the right/left arrow to go to next/previous parameter.

## Set Low CO<sub>2</sub> Alarm Limit (tracking alarm)

The low CO<sub>2</sub> alarm limit is the deviation from the CO<sub>2</sub> setpoint which will cause a low CO<sub>2</sub> alarm. The setpoint is variable from 0.5% CO<sub>2</sub> below setpoint to 5.0% CO<sub>2</sub> below setpoint. The factory setting is 1.0% CO<sub>2</sub> below setpoint. A minus sign (-) in the display indicates that the alarm setting is below the setpoint.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until CO<sub>2</sub> LO -X.X shows in the message display.
3. Press up/down arrow to change the low CO<sub>2</sub> alarm limit.
4. Press ENTER to save the low CO<sub>2</sub> alarm limit.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

## Set High CO<sub>2</sub> Alarm Limit (tracking alarm)

The high CO<sub>2</sub> alarm limit is the deviation from the CO<sub>2</sub> setpoint which will cause a high CO<sub>2</sub> alarm. The setpoint is variable from 0.5% CO<sub>2</sub> above setpoint to 5.0% CO<sub>2</sub> above setpoint. The factory setting is 1.0% CO<sub>2</sub> above setpoint.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until CO<sub>2</sub> HI X.X shows in the message display.
3. Press up/down arrow to change the high CO<sub>2</sub> alarm limit.
4. Press ENTER to save the high CO<sub>2</sub> alarm limit.
5. Press the MODE key to return to RUN mode, or right/left arrow to go to next/previous parameter.

## Enable CO<sub>2</sub> Alarms to Trip Contacts

High and Low CO<sub>2</sub> alarms can be programmed to trip the remote alarm contacts. A setting of ON allows this, a setting of OFF blocks CO<sub>2</sub> alarms from tripping the contacts. The factory setting is ON.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until CO<sub>2</sub> RLY XXX shows in the message display.
3. Press up/down arrow to toggle the setting ON/OFF.
4. Press ENTER to save the setting.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

## Set New Zero Number for T/C CO<sub>2</sub> Sensors

If a new T/C CO<sub>2</sub> sensor is being installed, the two numbers on the factory installed sticker on the T/C cell must be entered to calibrate CO<sub>2</sub> in the unit.

**Note** For the technician's convenience, a label containing the two numbers on the T/C cell is affixed inside the electronics drawer. ▲

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until T/CZ# XXXX shows in the message display.
3. Press up/down arrow to change the zero number to match the sticker.
4. Press ENTER to save the setting.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

## Set New Span Number for T/C CO<sub>2</sub> Sensors

If a new T/C CO<sub>2</sub> sensor is being installed, the two numbers on the factory installed sticker on the T/C cell must be entered to calibrate the CO<sub>2</sub> in the unit.

**Note** For the technician's convenience, a label containing the two numbers on the T/C cell is affixed inside the electronics drawer. ▲

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until T/CS# XXXX shows in the message display.
3. Press up/down arrow to change the span number to match the sticker.
4. Press ENTER to save the setting.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

## Setting a Low RH Alarm Limit

On units with the RH option installed, a low RH alarm limit may be entered. The low RH alarm limit is the %RH in the cabinet that causes a low RH alarm. The setpoint is variable from setpoint 0 to 90% RH. The factory setting is 0% RH, which disables the alarm.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until RH LO XX shows in the message display.
3. Press up/down arrow to change the RH low alarm limit.
4. Press ENTER to save the RH low alarm limit.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.

## **Enable RH Alarms to Trip Contacts**

The low RH alarm can be programmed to trip the remote alarm contacts. A setting of ON allows this, a setting of OFF blocks the RH alarm from tripping the contacts. The factory setting is ON.

1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until RH RLY XXX shows in the message display.
3. Press up/down arrow to toggle the setting ON/OFF.
4. Press ENTER to save the setting.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.


## **Enabling Temp/RH to be Displayed**

On units equipped with the RH option, the upper seven segment display on the control panel can be configured to display Temp continuously, RH continuously, or toggle between Temp and RH. If the units does not have RH, the upper display always shows temperature. If temperature is set to ON, and the RH is set OFF, temperature shows continuously. If temperature is set to OFF and RH is set to ON, RH shows continuously. If both are turned ON, the display toggles between the two. The factory setting defaults to toggle mode if the RH option is present.


1. Press the MODE key until the CON indicator lights.
2. Press the right arrow until DISP TMP XXX or DISP RH XXX shows in the message display.
3. Press up/down arrow to toggle the setting ON/OFF.
4. Press ENTER to save the setting.
5. Press the MODE key to return to RUN mode or right/left arrow to go to next/previous parameter.




# Chart 3-1. Configuration Mode Page 1 of 3

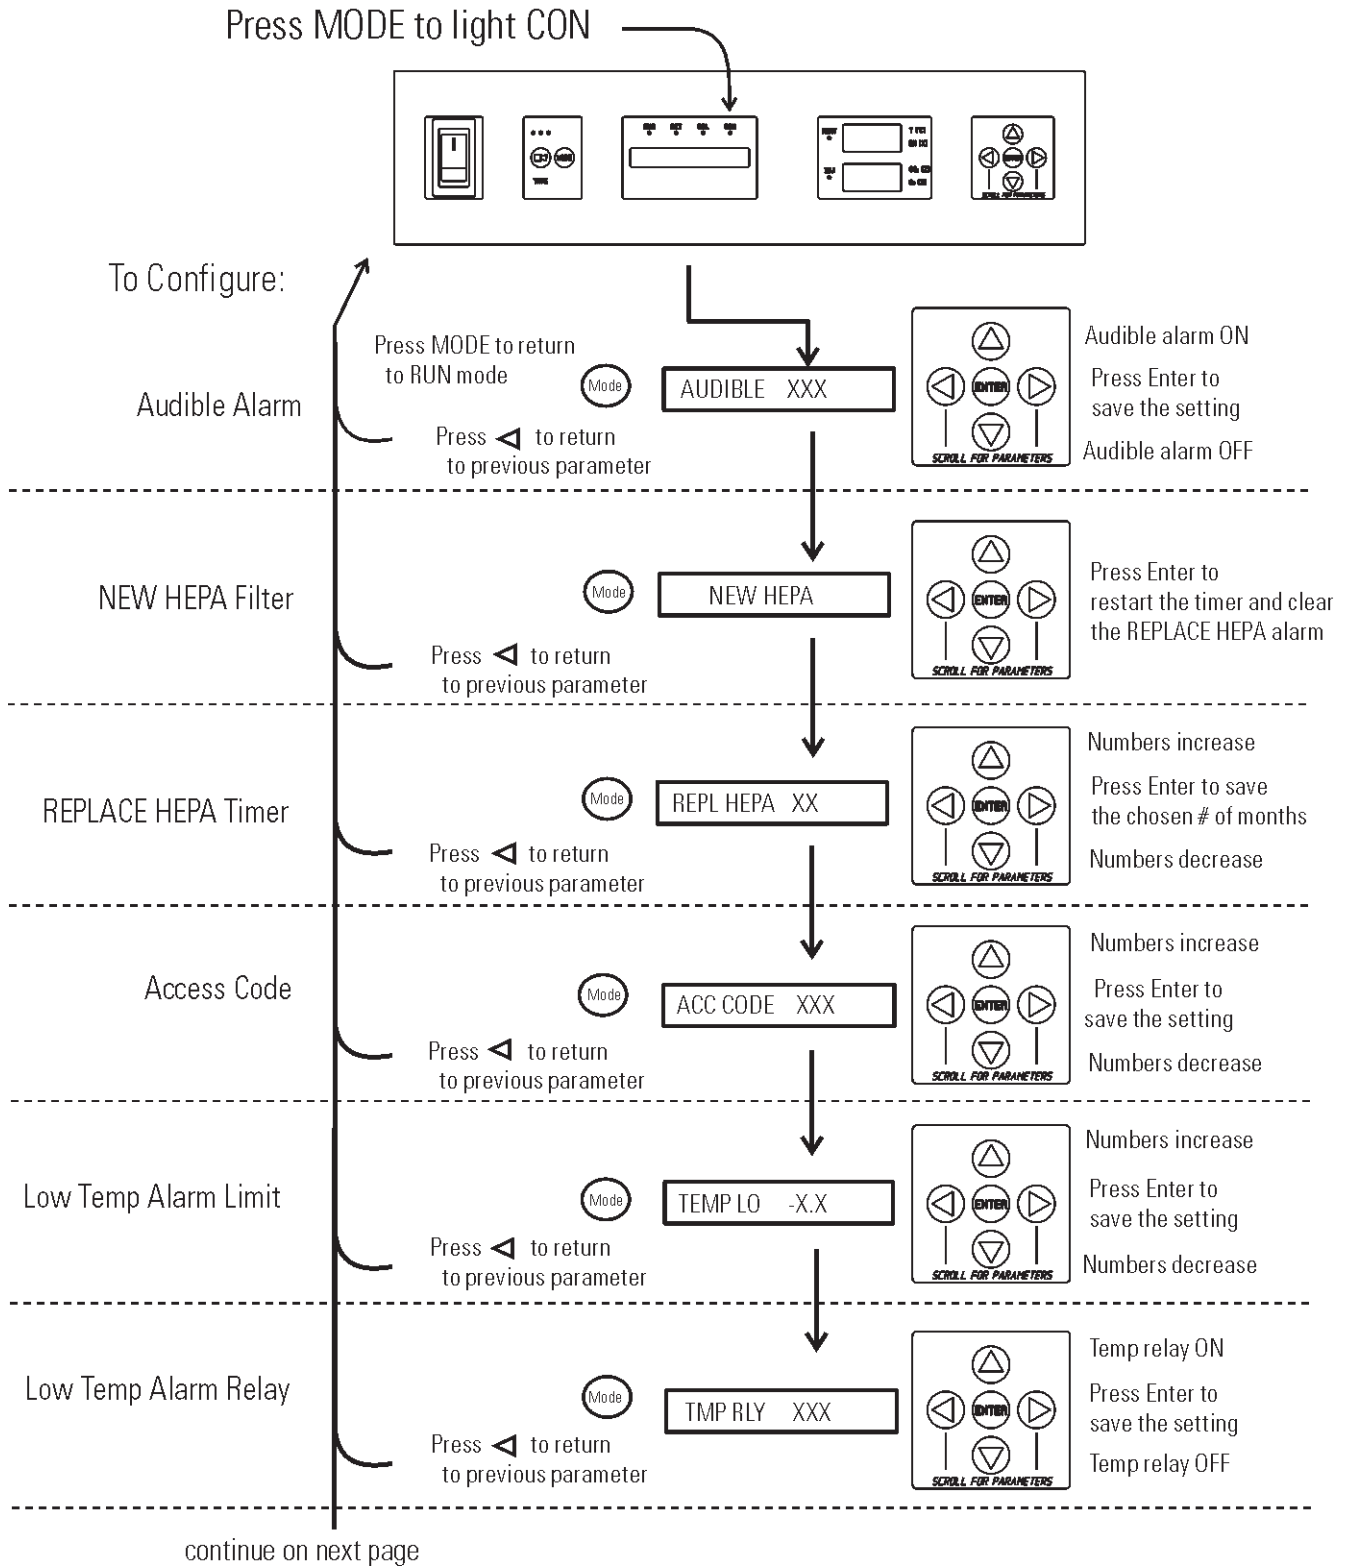


# Chart 3-1. Configuration Mode Page 2 of 3

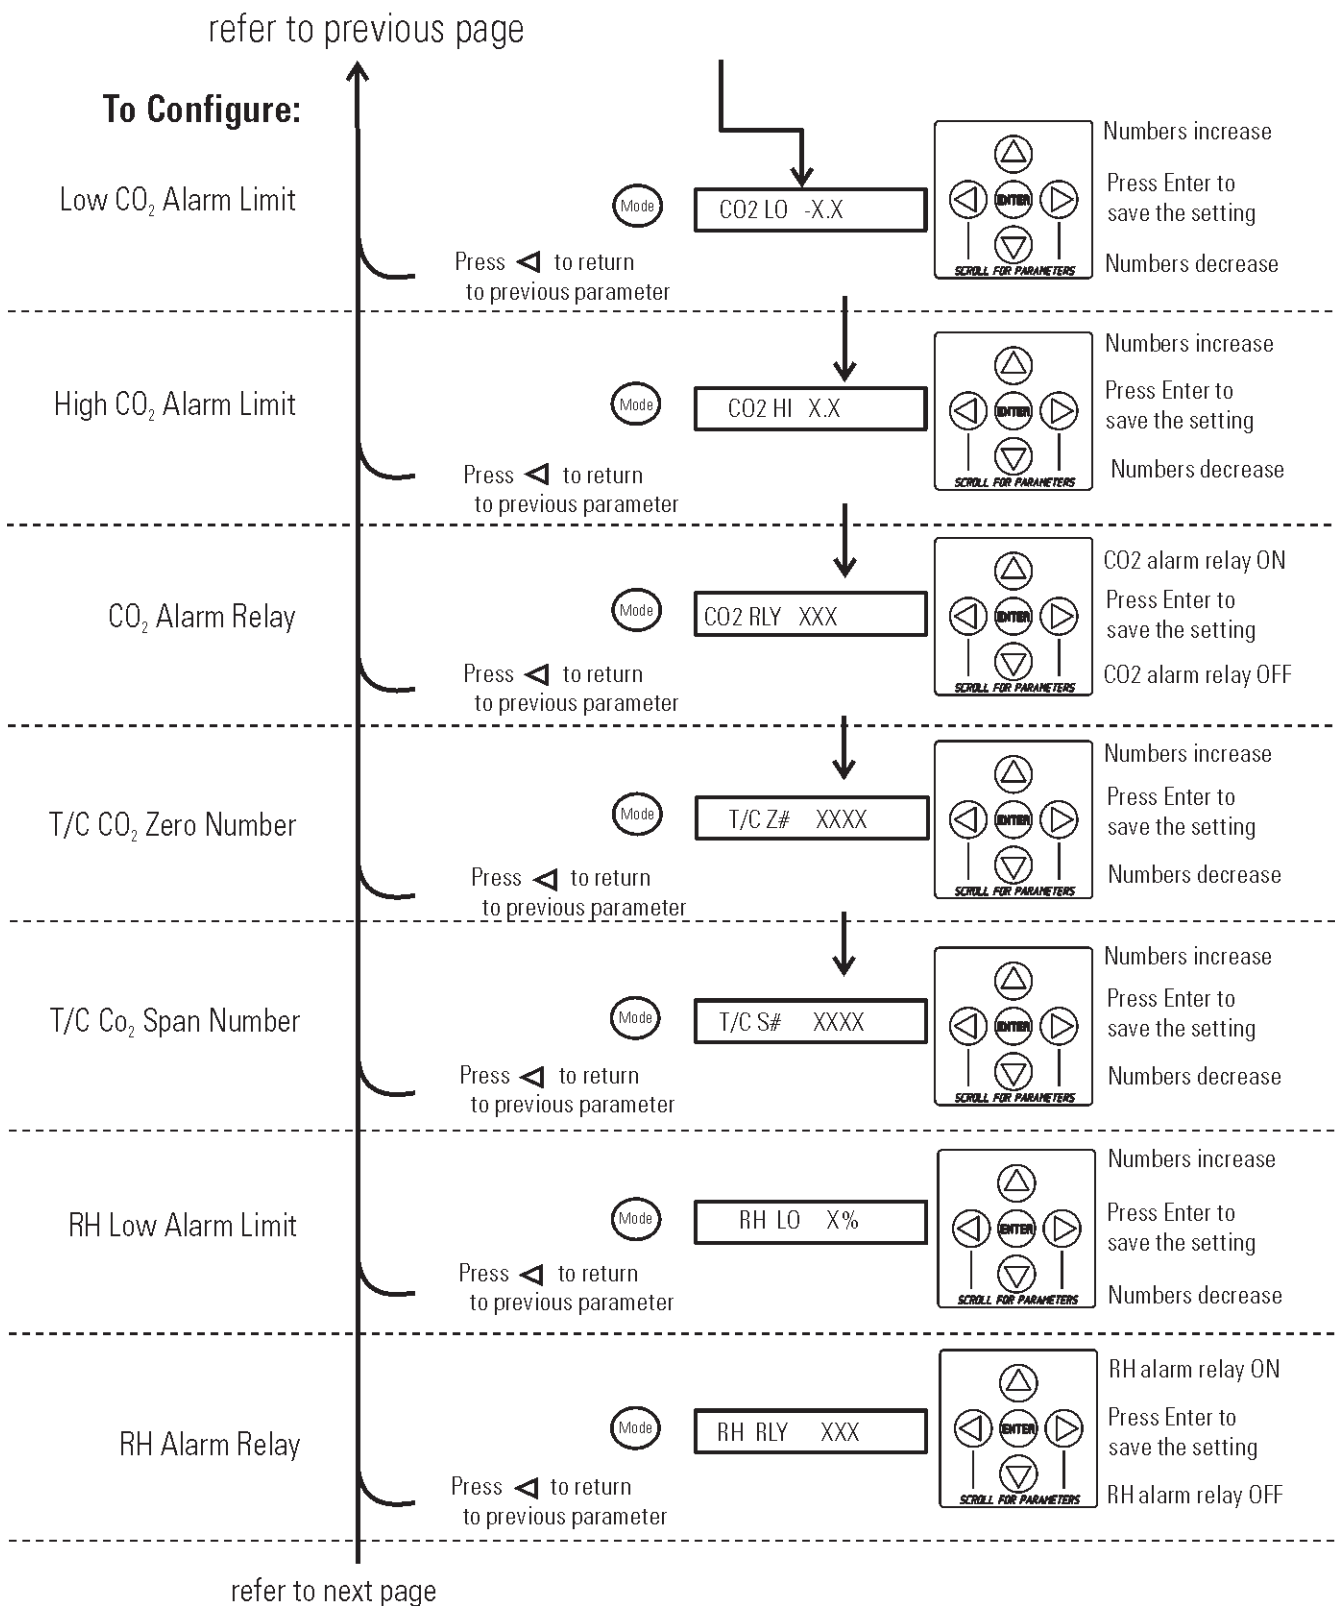

# Chart 3-1. Configuration Page 3 of 3

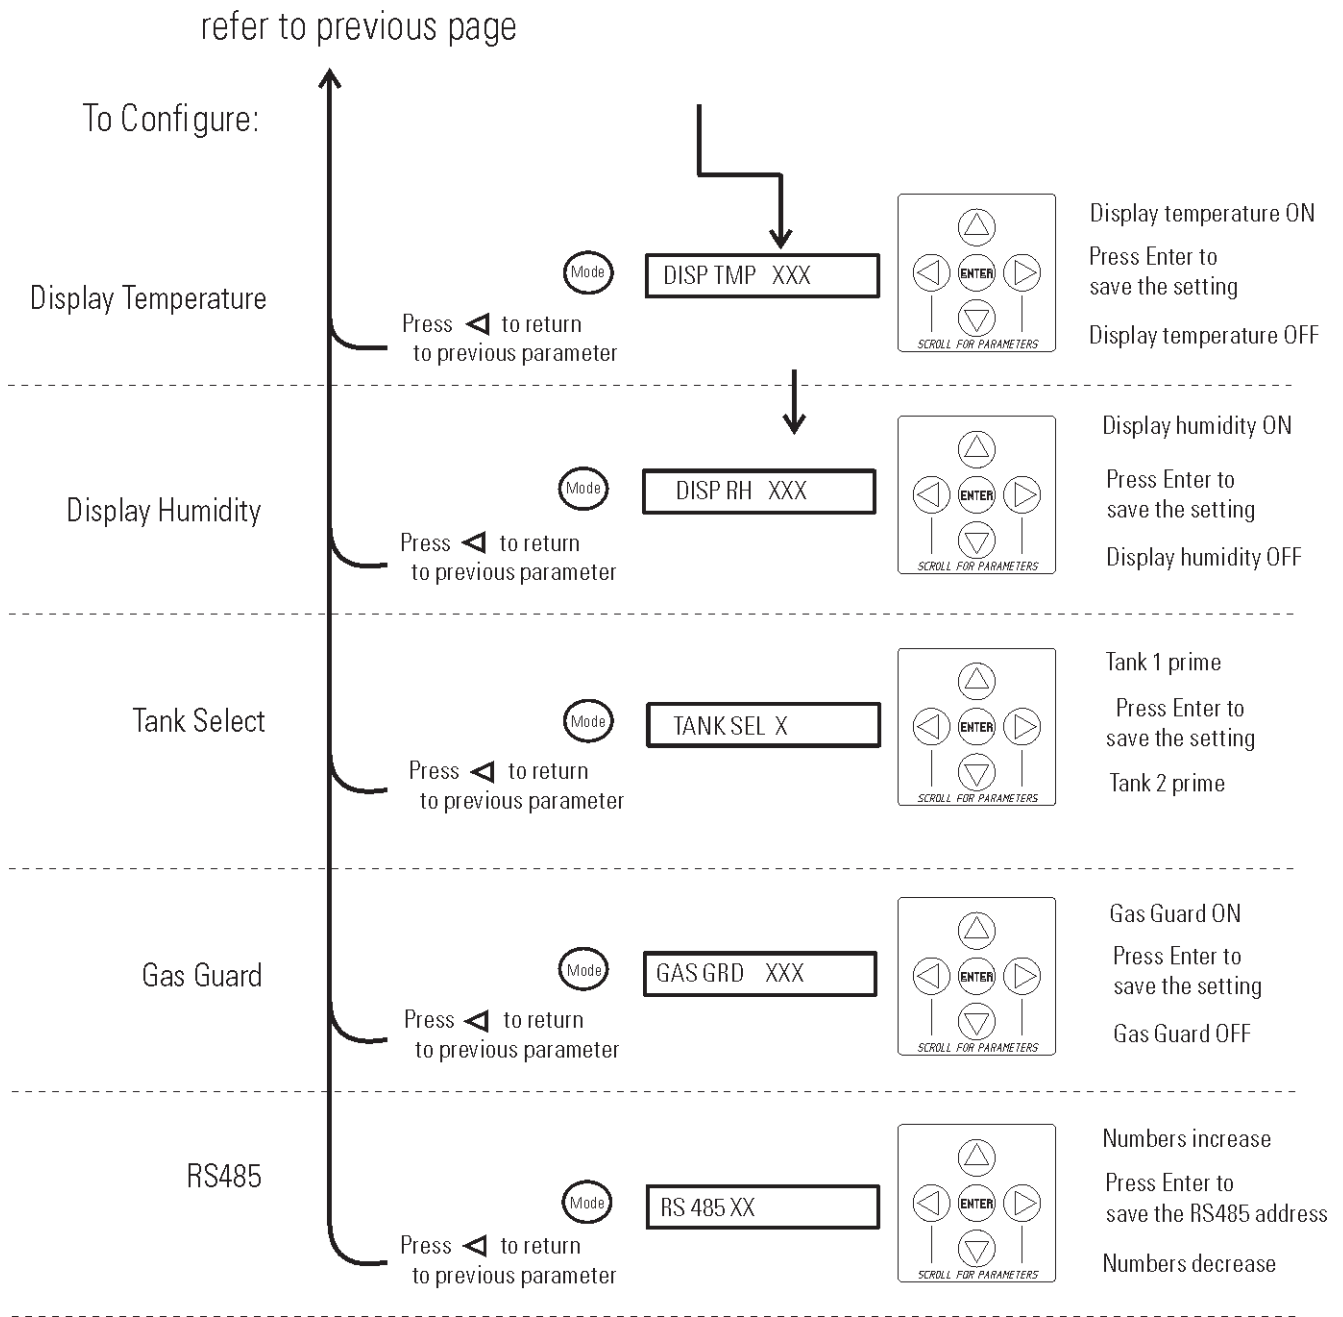


## Section 4 Alarms

The Series 8000DH incubator alarm system is shown in the table below. When an alarm is active, the message appears in the LED message display. Pressing  disables the audible alarm for the ringback period. However, the visual alarm continues until the incubator returns to a normal condition. The alarms are momentary alarms only. When an alarm condition occurs and then returns to normal, the incubator automatically clears the alarm condition and the message display.

**Table 4-1.** Alarm and Description

| Description   | Message                | Delay   | Ringback | Relay        |
|---|------------------------|---------|----------|--------------|
| No alarm condition exists                                     | SYSTEM OK or CLASS 100 | -----   | -----    | -----        |
| Temp > Otemp Set point  | SYS IN OTEMP           | 0 min.  | 15 min.  | Yes          |
| Air Temp Sensor Fault (See Section 4)                         | AIR SNSR ERR           | 0 min.  | 15 min.  | No           |
| Temperature Controller Failure (See Sect. 4)                  | TMP CTRL ERR           | 0 min.  | 15 min.  | YES          |
| CO2 Sensor Fault (See Section 4)                              | CO2 SNSR ERR           | 0 min.  | 15 min.  | No           |
| Replace HEPA filter reminder-set time expired (See Section 3) | REPLACE HEPA           | 0 min.  | -----    | No           |
| Inner Door is Open  | DOOR OPEN              | 15 min. | 15 min.  | No           |
| CO2 is higher than CO2 High Tracking Alarm                    | CO2 IS HIGH            | 15 min. | 15 min.  | Programmable |
| CO2 is lower than CO2 Low Tracking Alarm                      | CO2 IS LOW             | 15 min. | 15 min.  | Programmable |
| TEMP is lower TEMP Low Tracking Alarm                         | TEMP IS LOW            | 15 min. | 15 min.  | Programmable |
| RH is lower than RH Low Limit Alarm (RH option)               | RH IS LOW              | 30 min. | 15 min.  | Programmable |

- All alarm delays and ringback times are ±30 seconds -

When multiple alarm conditions occur, active messages are shown in the message display one at a time, updating at 5 second intervals. Pressing  during multiple alarms causes all active alarms to be silenced and to ring back in 15 minutes.

The TEMP IS LOW alarm is disabled when the Temp set point is 10°C. The CO<sub>2</sub> alarms are disabled when the CO<sub>2</sub> set point is 0.0%.

## **Temp Controller Failure TMP CNTR ERR**

In addition to other safety features designed into Series 8000DH incubators, a thermostat is provided to monitor the cabinet's temperature. In the unlikely event of a temperature control failure, the thermostat will turn off all heaters at a cabinet temperature of 160°C,  $\pm 5\%$ . This is intended to be a safety feature to protect the incubator, and is not intended to protect the cell cultures or the equipment inside the chamber should a temperature control failure occur. Should such a failure occur, contact the Technical Services Department or your local distributor.

## **Sensor Fault Alarms**

The microprocessor in Series 8000DH incubators continually scans all available sensors to ensure that they are operating properly. Should an error be detected, the incubator sounds an alarm and shows the appropriate message. Contact your local distributor.

# PREVENTIVE MAINTENANCE

## Incubators

Your equipment has been thoroughly tested and calibrated before shipment. Regular preventive maintenance is important to keep your unit functioning properly. The operator should perform routine cleaning and maintenance on a regular basis. For maximum performance and efficiency, it is recommended the unit be checked and calibrated periodically by a qualified service technician.

The following is a condensed list of preventive maintenance requirements. See the specified section of the operating manual for further details.

We have qualified service technicians, using NIST traceable instruments, available in many areas. For more information on Preventive Maintenance or Extended Warranties, please contact us at the number listed below.

Cleaning and calibration adjustment intervals are dependent upon use, environmental conditions and accuracy required.

### Tips for all incubators:

- Do NOT use bleach or any disinfectant that has high chloros
- Avoid spraying cleaner on the CO<sub>2</sub> sensor.
- Use sterile, distilled or demineralized water.
- Do not use powdered gloves for tissue cultures.

## Preventive Maintenance for Series 8000DH Incubators

| Refer to Manual Section | Action   | Daily | Weekly | Monthly | 3 to 6 Months | Yearly |
|-------------------------|--|-------|--------|---------|---------------|--------|
| --                      | Check CO <sub>2</sub> tank levels.   | ✓     |        |         |               |        |
| --                      | Inspect door latch, hinges and door gasket seal.   |       |        |         |               | ✓      |
| 1                       | Check water level in the humidity pan, 1/2" from top.  |       | ✓      |         |               |        |
| 2                       | Verify and document CO <sub>2</sub> , humidity and temperature calibration, as applicable (See Calibration).     |       |        |         |               | ✓      |
|                         | Disinfect the interior of the incubator (See Routine Maintenance).   |       |        |         | ✓             |        |
| 1                       | Replace HEPA, access port filter, air sample filter, and CO <sub>2</sub> filters*, if applicable (or as needed). |       |        |         |               | ✓      |
| 5                       | Perform sterilization cycle as needed.   |       |        |         |               |        |

## Section 5 Routine Maintenance

**Warning** If the unit has been in service, turn it off and disconnect the power cord connector before proceeding with any maintenance. ▲

**Caution** Before using any cleaning method except those recommended by the manufacturer, users must check with the manufacturer that the proposed method will not damage the equipment. ▲

Use an appropriate disinfectant. All articles and surfaces must be thoroughly cleaned, rinsed with sterile water, and rough-dried.


**Warning** Alcohol, even a 70% solution, is volatile and flammable. Use it only in a well-ventilated area that is free from open flame. If any component is cleaned with alcohol, do not expose the component to open flame or other possible hazard. Do not spray the T/C sensor with flammable solutions. The internal temperature of the CO<sub>2</sub> sensor is approximately 150°C when the unit is in operation. Allow sufficient time for the sensor to cool before cleaning.

Do not use strong alkaline or caustic agents. Stainless steel is corrosion resistant, not corrosion-proof. Do not use solutions of sodium hypochlorite (bleach) as they may also cause pitting and rusting. ▲

A HEPA filter replacement kit (see Parts List) should be on-hand prior to cleaning the incubator interior.



1. Remove the shelves, access port filter assembly, HEPA filter, air sample filter and tubing, and the left and right duct sheets. Discard the HEPA filters and the access port filter assembly. See Figure 5-1.

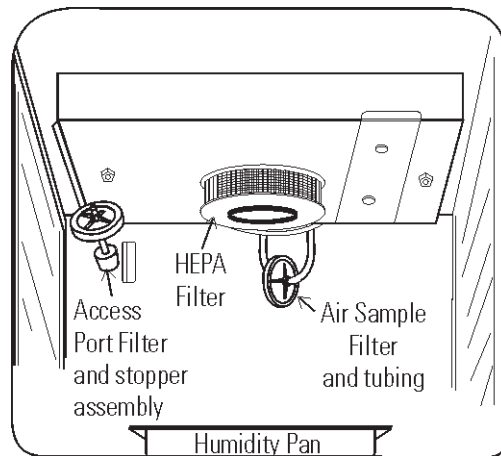

**Figure 5-1.** Component Locations

2. Wash the air sample filter tubing, shelves, and ducts with disinfectant, then rinse with sterile water. Optionally, the shelves and ducts may be autoclaved.
3. Wash the inner door gasket with disinfectant. This gasket may be removed to be cleaned, or replaced.
4. Wash the cabinet interior with disinfectant, starting at the top and working down. Refer to the disinfectant directions for length of time needed before rinsing. Wash the inner door both inside and out. The cabinet and door must be rinsed with sterile water until the disinfectant has been removed. After the cabinet has been rinsed, spray with 70% alcohol.
5. Install the left and right ducts, inner door gasket, access port filter assembly, and air sample filter and tubing, spraying each with 70% alcohol.
6. Install a new HEPA filter.
7. Install the shelves and spray with 70% alcohol.

## Clean Cabinet Exterior

Clean the incubator exterior with a damp sponge or soft, well-wrung cloth and mild detergent dissolved in water. Dry with a soft cloth.

## Clean Glass Doors

The chamber glass door and the optional independent inner glass doors may be cleaned using the same disinfectant as used on the incubator interior. It is imperative that they be rinsed with sterile distilled water to remove the disinfectant residue. The doors should then be dried with a soft cloth.

### Some precautions in the cleaning and care of the incubator glass doors:

Moisture leaches alkaline materials (sodium, Na) from the surface of the glass. Evaporation of the moisture concentrates the alkaline and may produce a white staining or clouding of the glass surface. Cleaning chemicals with a PH above 9 and heat (autoclaving) accelerate the corrosion process. Therefore, it is very important to rinse and dry the glass doors after cleaning. Autoclaving the glass doors should be avoided.

There is no simple method for repairing corroded glass. In most cases, the glass must be replaced.

## Clean Humidity Pan

Clean the humidity pan with soap and water and a general-use laboratory disinfectant. Rinse with sterile water and spray with 70% alcohol. The pan may be autoclaved.

## HEPA Filter Maintenance

Replace the HEPA filter when the REPLACE HEPA reminder is displayed. The REPLACE HEPA reminder can be set to alarm after a specified time from 1 to 12 months. The reminder default is the factory recommended setting of 6 months. For details, see Section 3.

## Replace Power Fuses

To access the only replaceable fuse in the incubator:


1. Turn off the incubator's power switch and unplug the power cord.
2. Remove the two screws from the top of the control panel. Grasp the control panel on each side and pull straight outward.
4. Figure 5-3 shows the location of the fuse. See Table 5-1 following for replacement fuse specifications.
5. Secure the control panel and return the unit to service. If the fuse blows after restoring power to the incubator, contact your local distributor.

**Table 5-1.** Fuse Replacement Chart

| Fuse Voltage | Manufacturer's P/N | Amperage Rating | Rupture Speed | IEC Letter Code |
|--------------|--------------------|-----------------|---------------|-----------------|
| 230VAC       | BUSS GMC-0.5A      | 500mA           | Time-Lag      | T               |
| 115VAC       | BUSS GMC-1.0A      | 1.0 Amp         | Time-Lag      | T               |

## Replace Air Sample Filter

1. Connect one end of the air sample filter to the hose barb on the chamber ceiling.
2. Connect the other end of the filter to the metal tubing on the HEPA filter adapter (Figure 5-2).

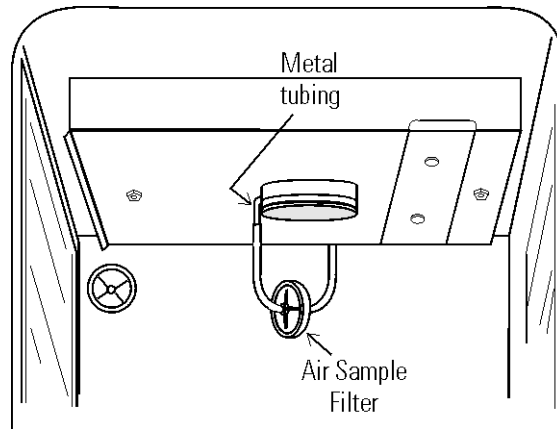


**Figure 5-2.** Connect to Metal Tubing

## Electronics Section

1. Turn off the incubator's power switch and unplug the power cord.
2. Remove the three screws from the back of the cabinet top.
3. Slide the top backward about an inch and lift it off.

## Major Components

Refer to Figure 5-3. Some components shown are factory installed options.

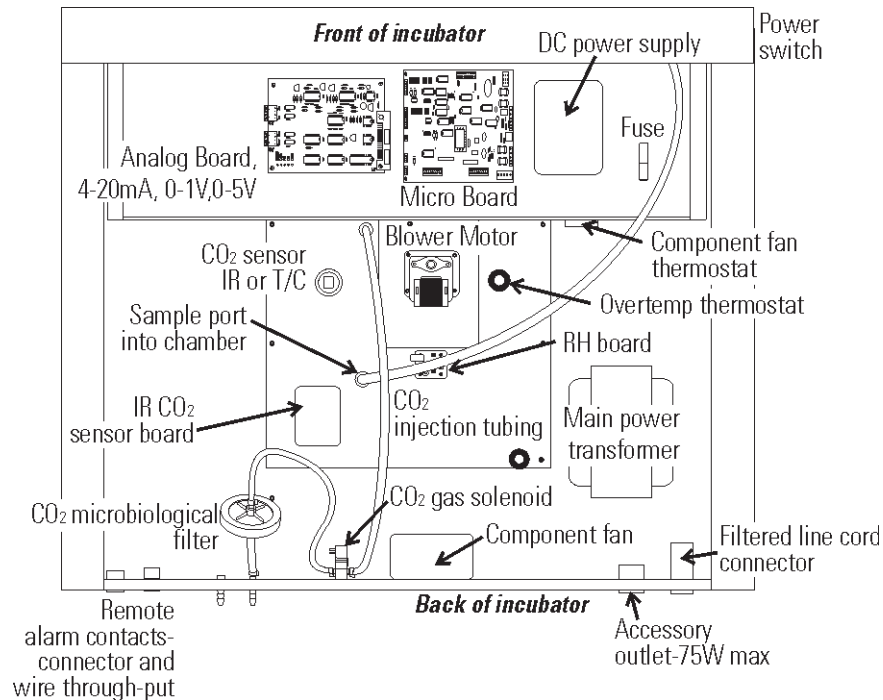

**Figure 5-3.** Electronics Drawer

## Sterilization Cycle

### Information You Need to Know Before Starting a Cycle


- The Sterilization Cycle requires approximately 12 hours - heat-up (2-4 hours), sterilize (2 hours), and cool down (6-8 hours). Additional time is needed to verify the calibration of temperature and CO<sub>2</sub> after the cycle is complete.
- During the Sterilization Cycle, the incubator updates the temperature to the analog output board and the 1535, however CO<sub>2</sub> will be fixed at setpoint and RH will be fixed at RH Low Limit plus 1%.
- A HEPA filter replacement kit (see the spare parts list) should be on hand prior to initiating the Sterilization Cycle.

### Information About the Cycle

- Pre-cleaning may be required. In order to avoid odors, stains on the interior, baked-on material, etc., wipe off all visible signs of spills.
- Odor may occur during the Sterilization Cycle and is considered normal.
- The Steri Cycle is not intended to sterilize other items; instruments, etc., from the lab.
- During the cycle, the unit chamber becomes hot enough to melt samples, instruments, dishes, etc., left inside the unit. The items listed below also need to be removed.

- 1) HEPA filter
- 2) Air sample filter
- 3) Access port filter assembly
- 4) Water in the humidity pan
- 5) Temp/RH recorder probe, if applicable
- 6) IR sensor, if applicable

- During the Sterilization Cycle, discoloration of some materials may occur. For example, stainless steel turns a straw color after a period of exposure to high temperatures. This is normal.

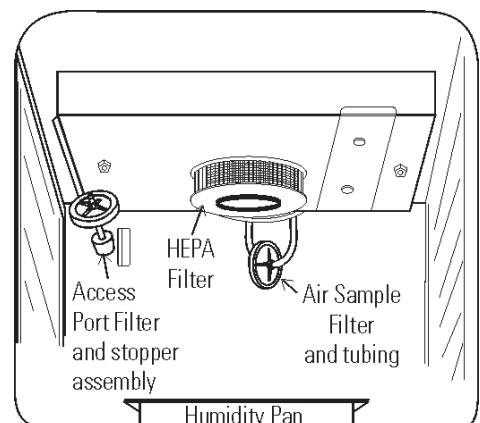

### Checkpoints


| <b>What if?</b>  | <b>Then</b>   |
|--|---|
| Cycle does not initiate or terminates in mid-cycle                                 | Check for alarms: SYS IN OTEMP, AIR SNSR ERR, TMP CTRL ERR  |
| Units are stacked  | A Sterilization Cycle performed on either unit affects performance on second unit.. Do not use second unit during Sterilization Cycle. The Sterilization Cycle may be performed on both units simultaneously, with proper electrical connection.  |
| No action is taken within 1 minute, following display prompt                       | Unit returns to normal operation, SYSTEM OK   |
| Need to cancel cycle in progress   | Hold down green cycle initiation button for 3 seconds   |
| Water is not removed from humidity pan during cycle                                | Steam is produced and may cause burns   |
| Listed components are not removed before initiating cycle                          | Components cannot withstand the sterilization cycle temperatures and are destroyed  |
| Unit is not powered off before removing the I/R sensor, if applicable              | Damage to the sensor may result   |
| Dummy I/R sensor is not installed  | The sensor cable cannot withstand sterilization cycle temperatures and is destroyed properly  |
| The outer door is opened during the heat or sterilization phases                   | An outer door alarm occurs: CLOSE DOOR in the display, plus an audible (cannot be silenced) and visual alarm.   |
| The outer door is open longer than 20 seconds during phases listed above           | Cycle is canceled, unit goes to CANCELED COOL PHASE*  |
| The outer door is open during the cool down phase when the temp is 60°C or greater | An outer door alarm occurs  |
| Power interruption during the HEAT PHASE   | HEAT PHASE resumes if the chamber temperature was less than 90°C when power was interrupted<br>HEAT PHASE resumes if the chamber temperature was greater than 90°C when power was interrupted, and the temperature dropped less than 1°C<br>CANCELED COOL PHASE* starts if the chamber temp drop is more than 1°C |
| Power interruption during the STERILIZATION PHASE                                  | HEAT PHASE begins if the chamber temperature has not dropped below 139°C<br>STERILIZATION PHASE starts again when the chamber temperature reaches 140°C<br>CANCELED COOL PHASE* starts if the chamber temp dropped below 139°C  |

\* For further information on CANCELED COOL PHASE, see page 5-12.

## Sterilization Cycle


**Warning** The Sterilization Cycle heats the incubator interior surfaces to 140°C. Contact with any surface inside the outer door during this cycle may result in burns. ▲

1. Empty the water from the humidity pan and place the pan back into the incubator. Remove any samples, instruments, dishes, etc. from the chamber.
2. Press and hold the large white sterilization cycle button on the right side of the unit (Figure 5-4) for approximately 3 seconds until the LED lights.

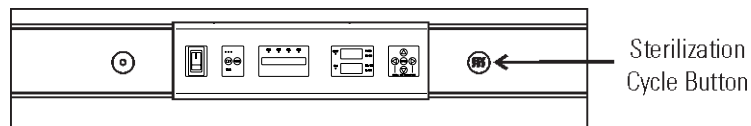

**Figure 5-4.** Sterilization Button Location


3. ENTER the access code, if applicable. An access code is recommended to prevent accidental cycle initiation.
4. **Pre Sterilization with T/C CO<sub>2</sub> sensor** - The display toggles between “REMOVE HEPAs”, “REMOVE WATER” and “PRESS ENTER”. If ENTER is not pressed within 1 minute, the display returns to “SYSTEM OK”.
5. Remove the HEPA filter, air sample filter and access port filter assembly (Figure 5-5). Tubing can remain in the unit during the sterilization cycle. In addition, remove the temp/RH recorder probe and IR sensor, if applicable. Discard the filters.

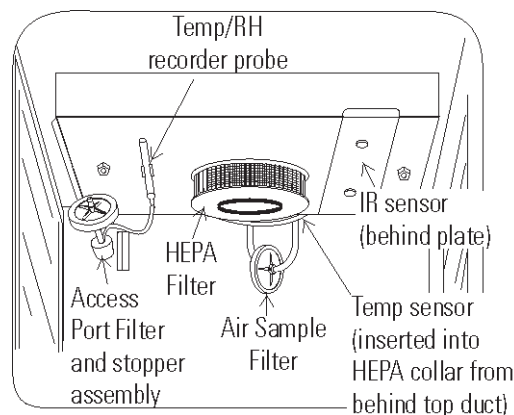


**Figure 5-5.** Filter Locations

**Pre Sterilization with IR CO<sub>2</sub> sensor** - If an IR sensor is connected, the display toggles between “POWER OFF” and “REMOVE IR”. If power is not turned off within 1 minute, the display returns to “SYSTEM OK”.

**Note** To remove the IR sensor, if applicable, first power the unit off. Then turn the two 1/4-turn fasteners on the top duct until the cover plate is disengaged. Secured on the inside of the plate is a dummy sensor (Figure 5-6). ▲

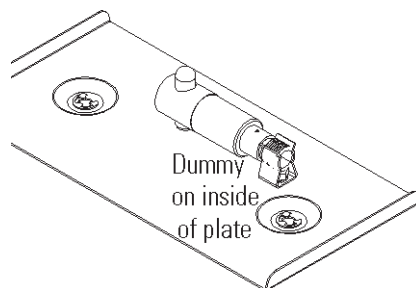


**Figure 5-6.** Dummy Sensor

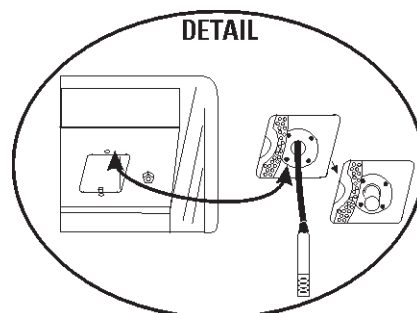

**Figure 5-7.** IR Sensor with Cable

Grip the IR sensor and carefully pull it downward. Unscrew the cable from IR sensor (Figure 5-13). Set the sensor aside. See Step 9 for the IR sensor disinfection procedure. Connect the dummy sensor to the cable. Fit the installed dummy sensor up into the previous sensor location.

When the power is turned on with the IR sensor removed, the display toggles between “REMOVE HEPAs”, “REMOVE WATER”, and “PRESS ENTER”. If “ENTER” is not pressed within 1 minute, the display toggles between “POWER OFF” and “REPLACE IR”. When the unit is powered back on with the IR sensor reinstalled, the display returns to “SYSTEM OK”.

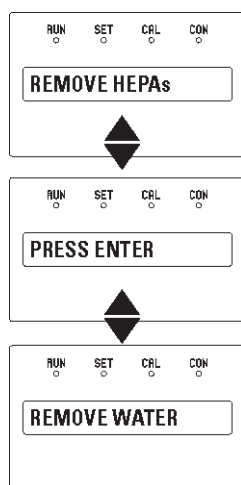

**Figure 5-14.** Displays with IR Sensor Removed



6. After ENTER is pressed, the Heat Phase initiates. The white LED flashes and the display toggles between “STERILIZING” and “HEAT PHASE”. During this period, the HEAT light will be on and the cabinet heats to sterilization temperature.

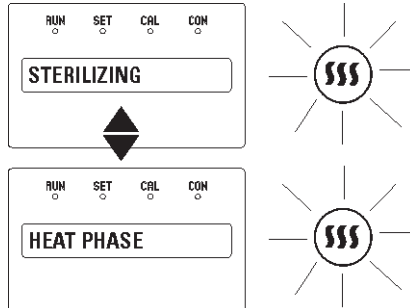


Figure 5-15. Heat Phase

7. When the air temperature in the unit reaches 140.0°C, the Sterilization Phase begins and the display changes to “STERILIZING”.

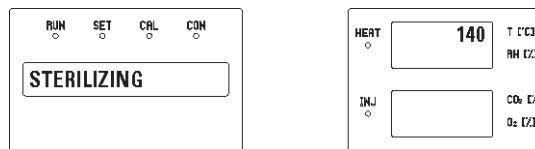


Figure 5-16. Sterilization Phase

8. After approximately 2 hours, a 5-second audible tone sounds, signaling that sterilization is complete. The Cool Phase begins. The display toggles between “STERILIZING” and “COOL PHASE”.

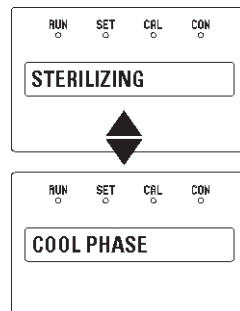


Figure 5-17. Cool Phase

9. **Completed Sterilization Cycle with T/C CO<sub>2</sub> sensor** - When the temperature cools down to the original set operating temperature or 30°C, whichever is higher, the display toggles between “CYC COMPLETE”, “REPL HEPAs”, and “PRESS ENTER”. The white LED is lighted but no longer flashes.


**Completed Sterilization Cycle with IR CO<sub>2</sub> sensor** - When the temperature cools down to the original set operating temperature or 30°C, whichever is higher, the display toggles between “CYC COMPLETE”, “POWER OFF”, and “REPLACE IR”. The white LED is lighted but no longer flashes.

Clean the IR sensor with either isopropanol or Lysol No-Rinse Sanitizer. When using isopropanol, simply spray the sensor (do not saturate) and allow to dry. With Lysol, spray the sensor (do not saturate) and allow to sit for a couple of minutes. Wipe dry with a clean, soft cloth.

**Do not saturate the sensor or immerse the sensor in a cleaner.**

Power the unit off, open the chamber, and remove the IR plate. Pull down on the dummy, unscrew the cable from the top of the dummy and press the dummy into the clip on the plate. See Figure 5-12. Screw the cable onto the top of the IR sensor. The cable is keyed and can only be inserted one way. Reinstall the sensor by pushing it as far as it will go into the hole.

After the unit is powered back on with the IR sensor reinstalled, the display toggles between “CYC COMPLETE”, “REPL HEPAs”, and “PRESS ENTER”.

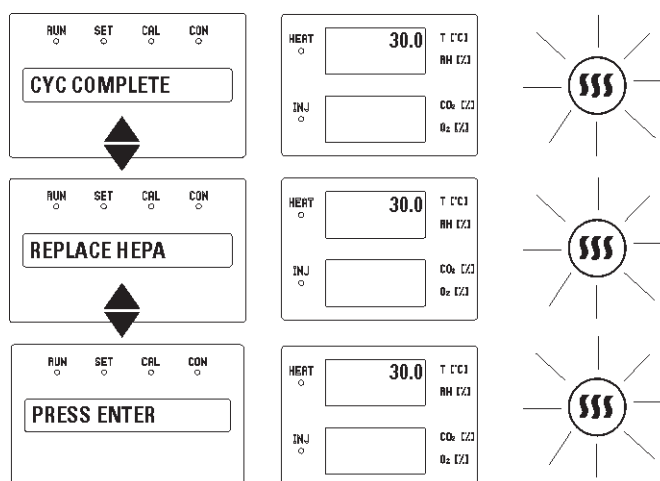

**Figure 5-18.** IR Sensor Reinstalled

10. Open the chamber and install a new HEPA filter, air sample filter and access port filter assembly. Press ENTER.
11. When ENTER is pressed, the LED goes out, the display returns to “SYSTEM OK”, and the HEPA filter replacement timer is reset.
12. Fill the humidity pan with 3 liters of sterile distilled water with the recommended purity range (See Section 1).
13. Allow to stabilize for at least 12 hours at the required temperature and CO<sub>2</sub> level. It is recommended that the temperature and CO<sub>2</sub> calibrations be verified periodically during the first week of returning the unit to service.

**Caution** The high temperature sterilization cycle may cause the T/C CO<sub>2</sub> sensor output to change significantly. (This is normal and does not indicate damage to the sensor.) Therefore it is essential that the CO<sub>2</sub> calibration is verified before returning the unit to service. ▲

If an independent instrument is not available to verify calibration, the following procedure may be performed. After the Sterilization Cycle and before CO<sub>2</sub> is allowed to enter the cabinet;

- 1) Fill and install the humidity pan.
- 2) Allow to stabilize at the desired operating temperature for at least 12 hours.
- 3) Calibrate the display to 0.0%.

**Note** If the Cool Phase is canceled, the display toggles between “CYC CANCELED” and “COOL PHASE”.

- With T/C CO<sub>2</sub> sensor - When the temperature cools down to the original set operating temperature or 30°C, whichever is higher, the display toggles between “CYC CANCELED”, “REPL HEPAs”, and “PRESS ENTER”. The white LED is lighted but no longer flashes.
- With IR CO<sub>2</sub> sensor - When the temperature cools down to the original set operating temperature or 30°C, whichever is higher, the display toggles between “CYC CANCELED”, “POWER OFF”, and “REPLACE IR”. The white LED is lighted but no longer flashes. After the unit is powered back on with the IR sensor reinstalled, the display toggles between “CYC CANCELED”, “REPL HEPAs” and “PRESS ENTER”.

## Section 6 Factory Options

A description of the factory option connections to external equipment follows.

### Remote Alarms

A set of relay contacts is provided to monitor alarms through an RJ11 telephone style connector on the back of the cabinet. Refer to Figure 6-5 for the location of the alarm connector. The 12-foot telephone cord (P/N 190388) and RJ11-to-screw terminal conversion box (P/N 190392) are available through your local distributor.

The remote alarm provides a NO (normally open) output, an NC (normally closed) output and COM (common). Refer to Figure 6-1.

The contacts will trip on a power outage or an overtemperature condition. The contacts may also be programmed to trip or not trip on temperature alarms, CO<sub>2</sub> alarms, and RH alarms. See Section 3, Configuration mode.

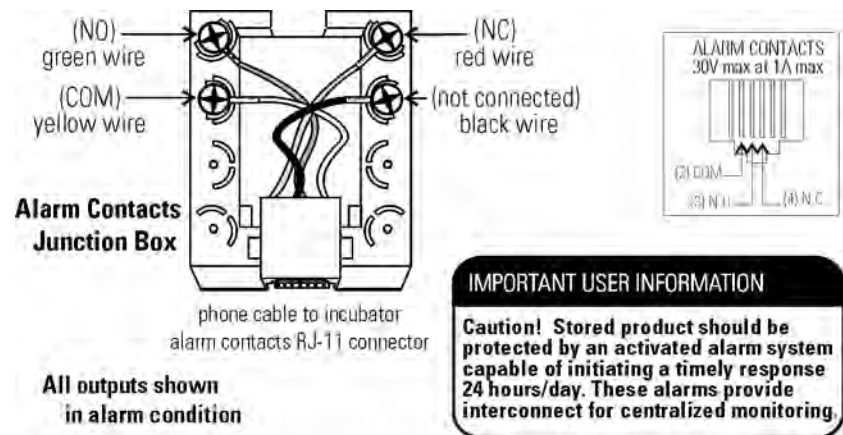


Figure 6-1. Remote Alarm Contacts



## Humidity Readout

Series 8000DH incubators are equipped with a humidity sensor to monitor the relative humidity inside the chamber. The sensor is located on the chamber ceiling and provides a signal that is displayed in 1% increments on the control panel. The humidity readout can display continuously, or toggle with the temperature readout. In addition, a low alarm limit can be set on the humidity readout to detect when the humidity pan runs dry. Refer to Section 3, Configuration.

The sensor is capable of measuring relative humidity from 10% to 100% with an accuracy of  $\pm 5\%$  above 90%. See Section 2, Calibration, for details on calibrating the humidity readout.

Factors which may affect humidity levels in the chamber are: the water level in the humidity pan, frequency of door openings, and the fact that the humidity pan is located on the bottom of the chamber versus on a shelf.

**Caution** Incubators equipped with a T/C (thermal conductivity) CO<sub>2</sub> sensor rely on a constant level of relative humidity to accurately measure and control the CO<sub>2</sub> concentration in the incubator. ▲

## Section 7 Specifications

\*Specifications are based on a nominal voltage of 115V or 230V in ambients of 22°C to 25°C.

### Temperature

Control . . . . . $\pm 0.1^\circ\text{C}$  Microprocessor PID Control  
Setpoint . . . . . Digital - Touch pad,  $0.1^\circ\text{C}$   
Range . . . . .  $+5^\circ\text{C}$  above ambient to  $50^\circ\text{C}$   
Uniformity . . . . .  $\pm 0.3^\circ\text{C}$  @  $+37^\circ\text{C}$   
Tracking alarm. . User programmable (low) indicator  
Overtemp . . Tracking, user programmable, action, and indicator  
Display . . . . . Digital, LED,  $0.1^\circ\text{C}$  increments

### Temperature Safety

Type . . . Extreme temperature safety, action, and indicator  
Sensor . . Thermostat, independent of temp control system  
Indicator . Message center, audible and visual alarms

### Relative Humidity

Control . . . . . Humidity pan - natural vaporization  
Humidity w/ pan . . . . . 95% RH at  $37^\circ\text{C}$   
Display . . . . . Optional in 1% increments  
Alarm . . . . . Low RH with optional RH monitor

### CO<sub>2</sub>

Control . . . . .  $\pm 0.1\%$  microprocessor PID control  
Sensor . . . . . T/C or IR  
Readability . . . . . 0.1%  
Range . . . . . 0 to 20%  
Inlet pressure . . . . . 15 psig (1 bar)  
Display . . . . . Digital LED, 0.1% increments

**Shelves**

Dimensions . . . . .18.5” x 18.5” (47cm x 47cm)  
Construction . . Stainless steel (belt sanded, both sides)  
Surface area . . . . .2.4 sq. ft. (0.22 sq. m.) per shelf  
Max. per chamber . . . . .38.4 sq. ft (3.6 sq. m.)  
Loading . . . 35 lbs (16kg) slide in and out, 50 lbs (23kg) stationary  
Standard . . . . .4  
Maximum . . . . .16

**Construction**

Interior volume . . . . .6.5 cu. ft. (184 liter)  
Interior . . . . .Type 304 stainless steel shiny finish  
Exterior . . . . .18 gauge cold roll steel  
Outer door gasket . . Four-sided molded, magnetic Santoprene  
Inner door gasket . . . . .Bulb, silicone  
Insulation . . . . .Mineral wool

**Fittings**

Access port . . 1-1/4” (32mm) removable silicone plug  
CO<sub>2</sub> inlet . . . . .1/4” (6.4mm) barbed  
Sample port . . . . .Front mounted barbed

**Electrical**

115 Volt models  
    . . . . .115VAC, 50/60 Hz, 1PH, 9.6 FLA  
    (Operating range 90-125VAC)  
230 Volt models  
    . . . . .230VAC, 50/60 Hz, 1 PH, 4.4 FLA  
    (Operating Range 180-250VAC)  
Power switch/circuit breaker . . . . 2 Pole, 12.0 Amp  
Accessory outlet . . .Voltage equal to the cabinet input.  
    75 Watts maximum, 0.5ma leakage current  
Alarm contacts . . .Deviation of temperature, CO<sub>2</sub>, power, NO and NC

**Dimensions**

- Exterior .....26.1" W x 39.5" H x 25.0" F-B  
 .....(66.3cm x 100.3cm x 63.5cm)
- Interior .....21.3" W x 26.8" H x 20.0" F-B  
 .....(54.0cm x 68.1cm x 50.8cm)

**Weight**

- Net .....260 lbs (118kg)
- Net shipping .....315 lbs (143kg)

**Certifications**

Refer to the Declaration of Conformity at the end of this manual

**Safety Specifications**

- Indoor Use Only
- Altitude .....2,000 meters
- Temperature .....5°C to 40°C
- Humidity .....80% RH at or below 31°C,  
 .....decreasing linearly to 50% RH at 40°C
- Mains Supply Fluctuations  
 Mains supply voltage fluctuations not to exceed ±10%  
 of nominal voltage
- Installation Category II<sup>1</sup>
- Pollution Degree 2<sup>2</sup>
- Class of Equipment<sup>1</sup>

---

1 Installation category (overvoltage category) defines the level of transient overvoltage which the instrument is designed to withstand safely. It depends on the nature of the electricity supply and its overvoltage protection means. For example, in CAT II which is the category used for instruments in installations supplied from a supply comparable to public mains such as hospital and research laboratories and most industrial laboratories, the expected transient overvoltage is 2500V for a 230V supply and 1500V for a 120V supply.

2 Pollution Degree describes the amount of conductive pollution present in the operating environment. Pollution degree 2 assumes that normally only non-conductive pollution such as dust occurs with the exception of occasional conductivity caused by condensation.






## Section 8 Spare Parts

| Part Number | Description   |
|-------------|---|
| 190699      | Removable feather gasket  |
| 190670      | Duct sheet and shelf channel kit  |
| 224175      | Stainless steel shelf   |
| 190884      | Stainless steel shelf and channels  |
| 191650      | Micro board, (main control)   |
| 230135      | Fuse, 1A, TD, 5 x 20mm (accessory outlet, 115V)                                 |
| 230120      | Fuse, 0.5A TD, 5 x 20mm (accessory outlet 230V)                                 |
| 430109      | Cordset, 10A, 250V  |
| 156117      | Motor, 2-pole, 115VAC, 50/60 Hz   |
| 190793      | Display board   |
| 290184      | Probe, 2252 Ohm/25°C, 1/8 x2  |
| 130077      | Stopper with 3/8" hole  |
| 290168      | Thermal conductivity (T/C) type CO <sub>2</sub> sensor                          |
| 231204      | Infrared type CO <sub>2</sub> sensor  |
| 250087      | CO <sub>2</sub> valve kit with assorted fittings                                |
| 965010      | CO <sub>2</sub> gas regulator   |
| 3166242     | Gas shuttle switch  |
| 3050        | External gas guard  |
| 950316      | Wall clamp for CO <sub>2</sub> bottle   |
| 231203      | RH sensor assembly (P/N 1900091 RH display option)                              |
| 230180      | 12A, DPDT circuit breaker switch (power)  |
| 400119      | Switcher, 40W, 12, 5, -12V  |
| 196018      | 34 position control to display ribbon cable                                     |
| 360239      | Inner door switch   |
| 360230      | Outer door switch   |
| 360236      | Sterilization initiation switch   |
| 100115      | Blower wheel  |
| 190985      | Access port filter assembly   |
| 760210      | Disposable in-line filters (10 filters)   |
| 770001      | Disposable filter, 99.97% (CO <sub>2</sub> line, air sample)                    |
| 760175      | HEPA filter, 5.5" diameter  |
| 760209      | HEPA value pack (4 filters)   |
| 1900067     | HEPA filter replacement kit   |
| 190650      | Independent inner door kit  |
| 190666      | Right hand door swing   |
| 1900063     | Roller base   |
| 140387      | Overlay   |
| 50109579    | AquaTec water cleaning cell 4-pack<br>(for water reservoirs, pans, and bottles) |
| 1900346     | Display control board   |

DWG. NUMBER: 370-200-2-B

| REV | ECN NO. | DATE     | BY  | CAD APPD | DESCRIPTION OF REVISION                |
|-----|---------|----------|-----|----------|--|
| 0   | N/A     | 4/10/01  | DCB | DNF      | RELEASE FOR PRODUCTION                 |
| 1   | IN-3308 | 06-30-08 | GJG | GJG      | MSB<br>ADDED NOTE #1                   |
| 2   | IN3759  | 01-22-07 | GJG | GJG      | CCS<br>ADDED COMMON TO FOR 8000 SERIES |

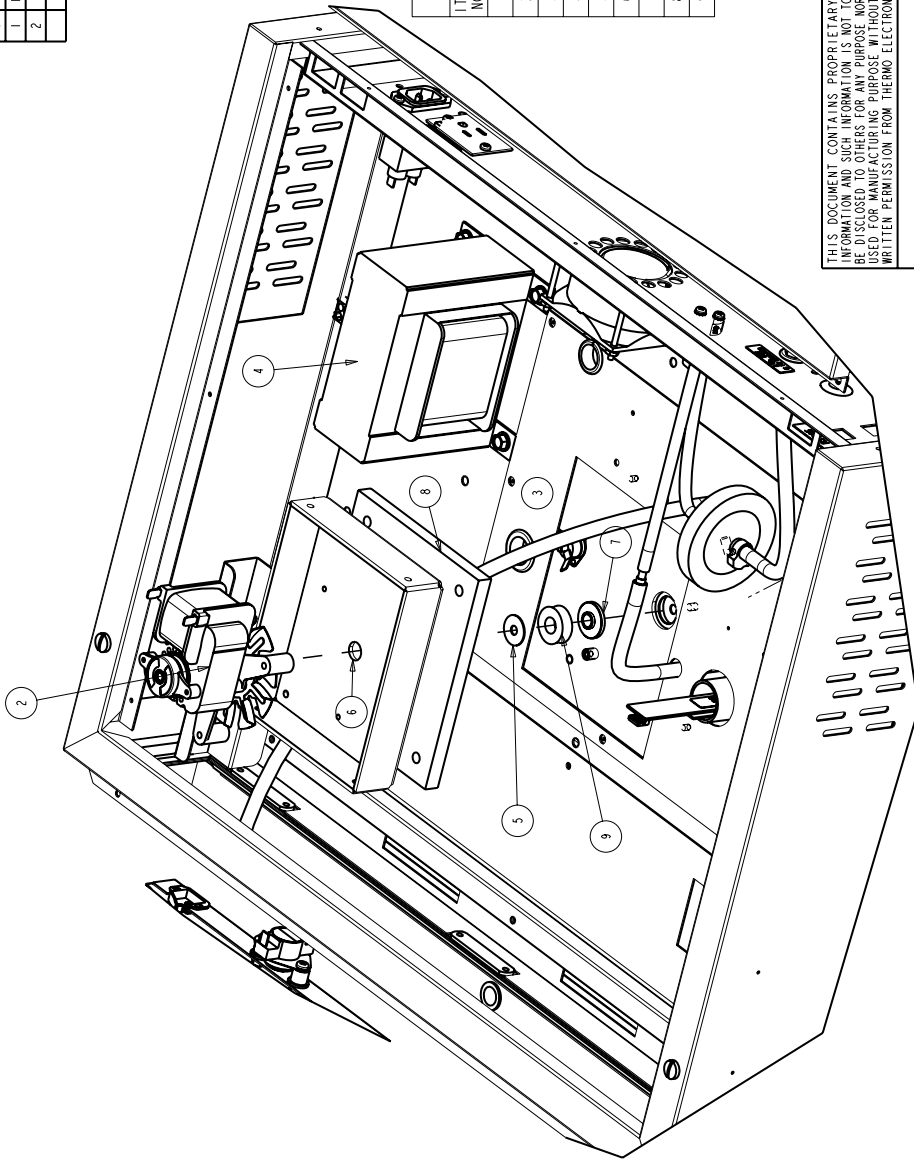

| BILL OF MATERIALS |            |                                 |     |
|-------------------|------------|---------------------------------|-----|
| ITEM NO.          | PART NO.   | PART DESCRIPTION                | QTY |
| 1                 | 23051      | #8-32 S. S. WING NUT            | 4   |
| 2                 | 156117     | BLOWER MOTOR                    | 1   |
| 3                 | 400150     | THERMOSTAT                      | 1   |
| 4                 | 420104     | 1 KVA TRANSFORMER               | 1   |
| 5                 | 730077     | TEFLON WASHER                   | 2   |
| 6                 | 1900302    | MOTOR MOUNT                     | 1   |
| 7                 | 1900315    | BLOWER SHAFT BUSHING            | 1   |
| 8                 | 140300_PT3 | BLOWER INSULATION 370 PART OF 3 | 1   |
| 9                 | 730069_370 | SILICONE WASHER                 | 1   |

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSE WITHOUT WRITTEN PERMISSION FROM THERMO ELECTRON

MODEL/PART NAME: 370 SERIES STERI-CYCLE INCUBATOR  
 DWG TITLE: ASSEMBLY  
 DWN: DALE CAD: DCB APPD: DNF DATE: 4/6/01 SCALE: 0.375  
 MATERIAL: -

PAINT: WHITE  
 TOLERANCE UNLESS OTHERWISE SPECIFIED: ANGLES: DECIMAL: .XX±  
 DRAWING NUMBER: 370-200-2  
 SIZE: B

**Thermo**  
 Fisher Scientific  
 Controls Environmental Equipment  
 Box 648, Marietta, Oh 45750

1. COMMON TO 3598, 3540, 3541, 3542, 3543

Dwg. NUMBER: 370-200-3-B


| REV | ECN NO. | DATE     | BY  | CAO  | APPD | DESCRIPTION OF REVISION                 |
|-----|---------|----------|-----|------|------|---|
| 0   | N/A     | 4/11/01  | DCB | DCB  | DNF  | RELEASE FOR PRODUCTION                  |
| 1   | IN-2942 | 05-14-01 | DCB | KDG  | LDN  | REMOVED TOP ROW OF TABS FROM DUCT SHEET |
| 2   | IN-3124 | 07-30-03 | JNL | KDG  | LDN  | CHANGED 290137 PROBE TO 290184          |
| 3   | IN-3306 | 06-30-06 | GJG | MSB  |      | ADDED NOTE #1                           |
| 4   | IN-3759 | 01-22-07 | GJG | LCCS |      | ADDED COMMON TO FUR 6000 SERIES         |

| ITEM NO. | PART NO.     | PART DESCRIPTION                 | QTY |
|----------|--------------|----------------------------------|-----|
| 1        | 23004        | 1/4-20 SS HEX NUT                | (4) |
| 2        | 101013       | 3" SILICONE O-RING               | 1   |
| 3        | 190723       | MODULAR W/J DUCT SHEET           | 2   |
| 4        | 224175       | INC. SHELF - 2B BRUSHED BACK     | 1   |
| 5        | 237016       | HUMIDITY PAN                     | 1   |
| 6        | 760175       | 5-500" HEPTA FILTER              | 1   |
| 7        | 770001       | DISPOSIBLE HEPTA FILTER 1/4 (B)  | 1   |
| 8        | 1900097      | ACCESS PLATE                     | 1   |
| 9        | 1900311      | 370 SERIES TOP DUCT SUB-ASSEMBLY | 1   |
| 10       | 1900308-31-1 | EXTERIOR TOP SHELF CHANNEL       | 1   |
| 11       | 190664-31-1  | TEMPERATURE SENSOR               | 2   |
| 12       | 290184       | TEMPERATURE SENSOR               | 1   |
| 13       | FLTRD_AIR_2  | 244020 SILICONE TUBE 6"          | 1   |
| 14       | FLTRD_AIR_3  | 244020 SILICONE TUBE 5"          | 1   |

**BILL OF MATERIALS**



THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSES WITHOUT WRITTEN PERMISSION FROM THERMO FISHER SCIENTIFIC

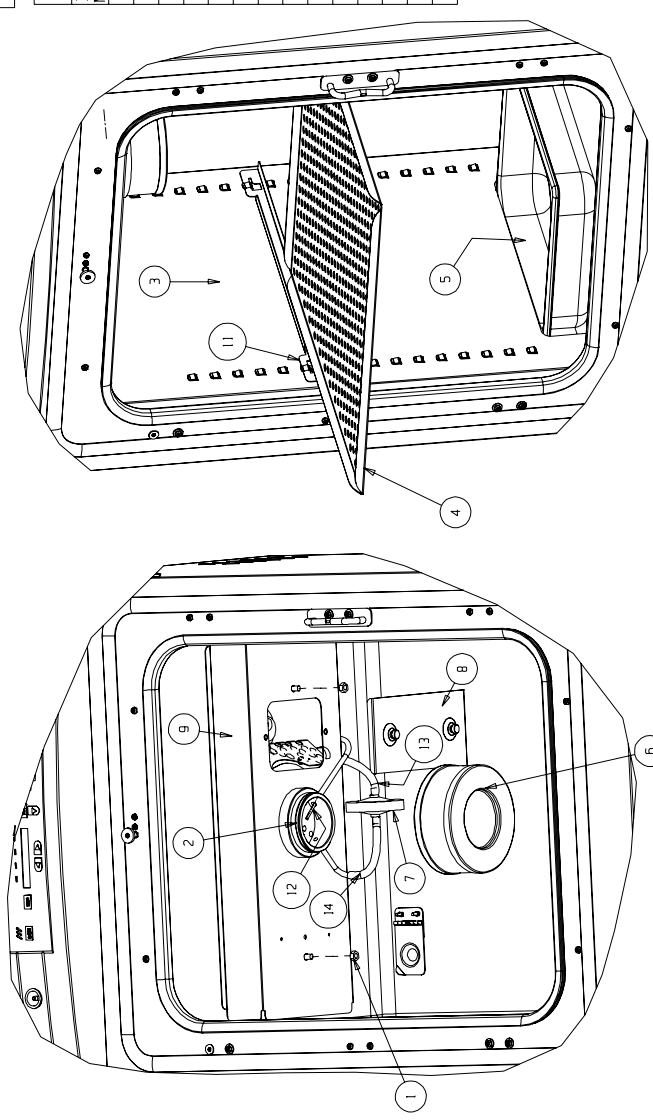**ThermoFisher**  
**SCIENTIFIC**

BDX 646, MARIETTA, OHIO 45750

MODEL/PART NAME: 370 SERIES STERILE-CYCLE INCUBATOR

DWG TITLE: ASSEMBLY

DNW: DNE    CAD: DCB    APPD: DNF    DATE: 4/6/01    SCALE: 0.200

MATERIAL: -

PAINT: WHITE

TOLERANCE UNLESS OTHERWISE SPECIFIED  
DECIMAL: .XXX±

DRAWING NUMBER: 370-200-3


SIZE: B

1. COMMON TO 359B, 3540, 3541, 3542, 3543

DWG. NUMBER: 370-200-4-B

| REV | ECN NO. | DATE     | BY  | CAD | APPO | DESCRIPTION OF REVISION     |
|-----|---------|----------|-----|-----|------|-----------------------------|
| 0   | N/A     | 4/11/01  | DCB | DNF |      | RELEASED FOR PRODUCTION     |
| 1   | IN-3306 | 06-30-06 | GJG | MSB |      | ADDED NOTE#1                |
| 2   | IN-3759 | 01-22-07 | GJG | ECS |      | ADDED COMMON TO 8000 SERIES |

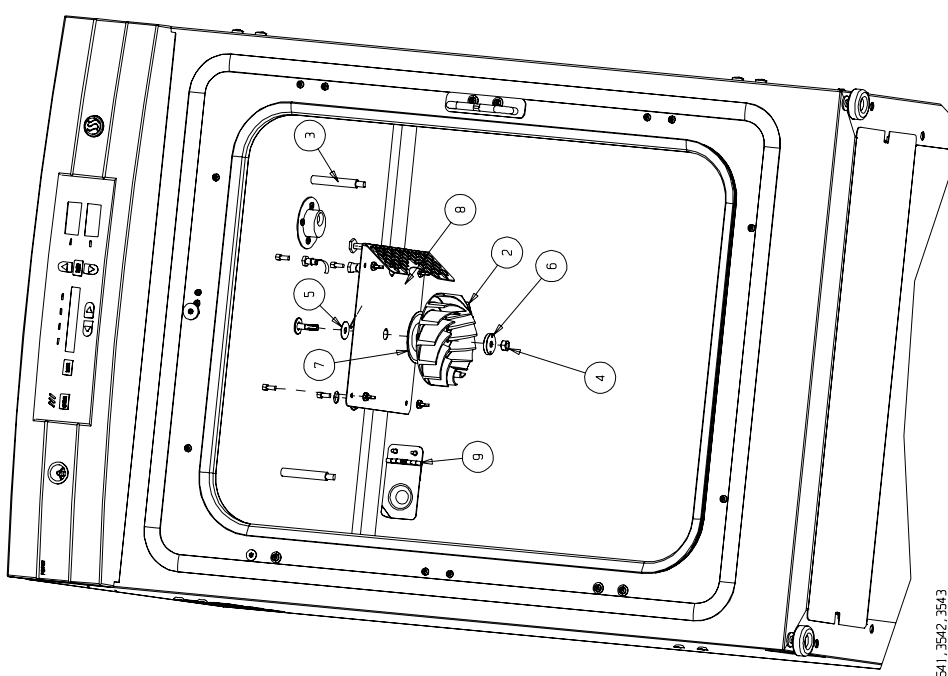

**BILL OF MATERIALS**

| ITEM NO. | PART NO.   | PART DESCRIPTION           | QTY |
|----------|------------|----------------------------|-----|
| 1        | 23051      | #8-32 S.S. WING NUT        | 4   |
| 2        | 100115     | VORTEX BLOWER WHEEL CW     | 1   |
| 3        | 127066     | 2.250" SPACER 1/4"-20      | 2   |
| 4        | 610075     | 1/4"-20 SS LEFT-HANDED NUT | 1   |
| 5        | 730077     | TEFLON WASHER              | 2   |
| 6        | 1900083    | BRASS FAN ADAPTER          | 1   |
| 7        | 1900111    | BLOWER WHEEL PLATE         | 1   |
| 8        | 1900320    | CLASS 100 PLATE            | 1   |
| 9        | 1900322    | ACCESS PORT FLAP ASSEMBLY  | 1   |
| 10       | 290184_370 | TEMPERATURE SENSOR         | 1   |

|   |          |           |              |
|---|----------|-----------|--------------|
| MODE/PART NAME: 370 SERIES STERIL-CYCLE INCUBATOR |          |           |              |
| DWG TITLE: ASSEMBLY                               |          |           |              |
| DWG. DATE   | CAD. JOB | APPO. DNF | DATE: 4/6/01 |
| MATERIAL: -                                       |          |           | SCALE: 0.2/8 |
| PAINT: WHITE                                      |          |           |              |
| TOLERANCE UNLESS OTHERWISE SPECIFIED              |          |           |              |
| ANGLES:   | DECIMAL: | .XXX±     |              |
| DRAWING NUMBER                                    |          |           | 370-200-4    |
| SIZE  |          |           | B            |

**THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSES WITHOUT WRITTEN PERMISSION FROM THERMO FISHER.**

**Thermo**  
Fisher Scientific Corporation  
One Northpointe Drive  
Columbus, OH 43260-1099  
© 2007 Thermo Fisher Scientific Inc.


1. COMMON TO 3598, 3540, 3541, 3542, 3543

DWG. NUMBER: 370-200-5-B

| REV | ECN NO. | DATE     | BY  | CAD | APPD | DESCRIPTION OF REVISION              |
|-----|---------|----------|-----|-----|------|--------------------------------------|
| 2   | PIP-029 | 08-29-01 | NWC | PKD | KDG  | REVISED OUTLET MOUNT                 |
| 3   | SI-9181 | 05-19-04 | GLM | KGS | LDN  | CHG'D. 250085 CLIPPARD VALVE TO ASCO |
| 4   | IN-3306 | 06-30-06 | GJG | GJG | MSB  | ADDED NOTE #1                        |
| 5   | IN-3759 | 01-22-07 | GJG | GJG | LDN  | ADDED COMMON TO 800 SERIES           |
| 6   | IN-3824 | 12-12-07 | BJK | SAG |      | REMOVED STUD FROM BACK PANEL         |

BILL OF MATERIALS

| ITEM NO. | PART NO.        | PART DESCRIPTION                              | QTY |
|----------|-----------------|---|-----|
| 1        | 22011           | #6-32 x 2 SS PHP SCREW                        | 4   |
| 2        | 22049           | #6-32 x 3/8 SS PHP SCREW                      | 6   |
| 3        | 23001           | #6-32 ZP LWASH HEX NUT(3/80 ONLY)             | 4   |
| 4        | 23024           | 3/8" SS FLAT WASHER                           | 1   |
| 5        | 23058           | #6 SS EXT TOOTH LOCKWASHER                    | 2   |
| 6        | 34014           | 1/2" SWAP-IN HOLE PLUG (BLACK) 3711, 381 ONLY | 1   |
| 7        | 190994          | ACCESSORY OUTLET MOUNT                        | 1   |
| 8        | 220259          | ACCESS OUTLET LABEL                           | 1   |
| 9        | 220381          | ALARM CONTACT LABEL                           | 1   |
| 10       | 220490          | REFER TO MANUAL LABEL                         | 1   |
| 11       | 220565          | RS-485 LABEL                                  | 1   |
| 12       | 220566          | CO2 #1 LABEL                                  | 1   |
| 13       | 250085          | SOLENOID VALVE 12V                            | 1   |
| 14       | 460024          | SWAP-IN OUTLET, WHITE                         | 1   |
| 15       | 460138          | POWER OUTLET                                  | 1   |
| 16       | 460180          |   | 1   |
| 17       | 600034          | SWAPPER CLAMP .375                            | 3   |
| 18       | 600063          | SWAPPER CLAMP .312                            | 1   |
| 19       | 730044          | SHOULDER WASHER .375" ID                      | 1   |
| 20       | 710001          | DISPOSIBLE HEPIA FILTER 1/4                   | 1   |
| 21       | 840008          | 5/32 TUBING ADAPTER                           | 2   |
| 22       | 900135          | 3.15" SQUARE FAN                              | 1   |
| 23       | 1900313         | BACK PANEL                                    | 1   |
| 24       | 370-CO2-INLET-2 | 72015 3/16" VINYL TUBING 6"                   | 1   |
| 25       | 370-CO2-INLET-1 | 950013 VINYL INLET TUBE 370, 8"               | 1   |
| 26       | 840020-FTG      | 250 BULKHEAD FITTING                          | 1   |
| 27       | 840020-NUT      | .375 NUT BLKHD FITTING                        | 1   |
| 28       | 840020-WSHR     | .375 IT WASHER BLKHD FTG                      | 1   |

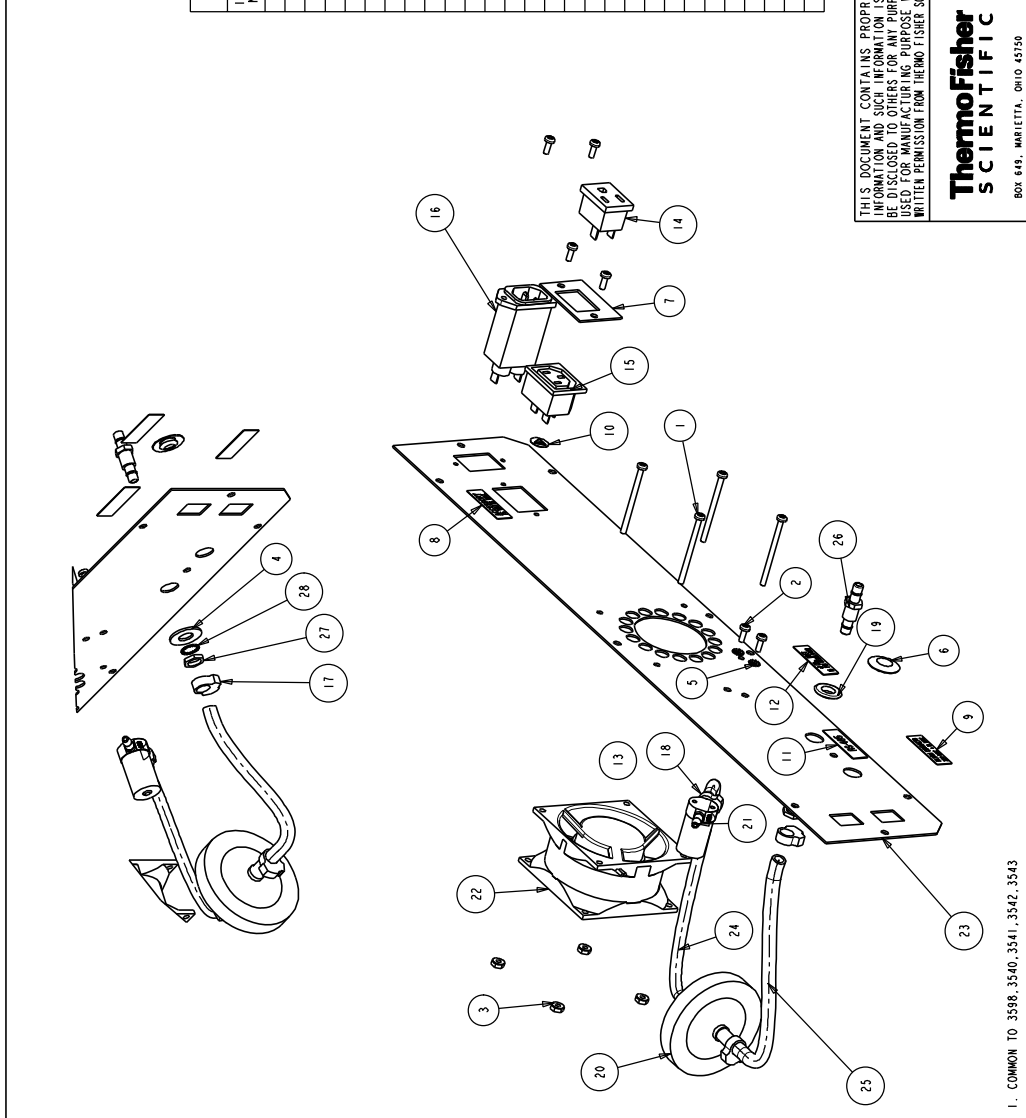

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED OR REPRODUCED FOR ANY USE WITHOUT THE EXPRESS WRITTEN PERMISSION FROM THERMO FISHER SCIENTIFIC

**ThermoFisher SCIENTIFIC**  
800 649, MARLETTA, OHIO 45359


|                                      |                |              |
|--------------------------------------|----------------|--------------|
| MODEL/PART NAME: 370 INCUBATOR       | DATE: 3/26/01  | SCALE: 0.375 |
| DWG TITLE: 370 BACK PANEL ASSEMBLY   | APPD: DNF      |              |
| DWN: DALE                            | CAD: DCB       |              |
| MATERIAL: -                          |                |              |
| PAINT: N/A                           |                |              |
| TOLERANCE UNLESS OTHERWISE SPECIFIED | DRAWING NUMBER | SIZE         |
| ANGLES: .XXX°                        | 370-200-5      | B            |

DWG. NUMBER: 370-200-6-B

| REV | ECN NO. | DATE     | BY  | CAD | APPD | DESCRIPTION OF REVISION           |
|-----|---------|----------|-----|-----|------|-----------------------------------|
| 0   | N/A     | 3/28/01  | DCB | DNF |      | RELEASED FOR PRODUCTION           |
| 1   | 1N-2994 | 10-25-01 | WCW | PKG | LDN  | CHG. FROM 22130 & 23029 TO 590032 |
| 2   | 1N-3048 | 09-25-02 | GJG | KOG | LDN  | ADDED (4) 515084 SPACERS          |
| 3   | 1N-3306 | 06-30-06 | GJG | GJG | LDN  | ADDED NOTE #1                     |
| 4   | 1N-3758 | 01-04-07 | WCW | KOG | LDN  | REMOVED (4) 610055 CLIP NUTS      |
| 5   | 1N-3759 | 01-22-07 | GJG | GJG |      | ADDED COMMON TO 8000 SERIES       |

**BILL OF MATERIALS**

| ITEM NO. | PART NO.     | PART DESCRIPTION                  | QTY |
|----------|--------------|-----------------------------------|-----|
| 1        | 22015        | #8-32 X 3/4 SS PHP SCREW          | 2   |
| 2        | 23002        | #8-32 ZP LKWASH HEX NUT           | 3   |
| 3        | 23006        | #4-40 ZP LKWASH HEX NUT           | 1   |
| 4        | 59007        | #4-40 X 3/8 SS PHP SCREW          | 1   |
| 5        | 111037       | NYLON WIRE SADDLE                 | 2   |
| 6        | 120048       | NYLON BEARING 1/4" X 7/16"        | 2   |
| 7        | 191650       | 370 SERIES INCUBATOR MICRO BOARD  | 1   |
| 8        | 220359       | 1 AMP FUSE LABEL                  | 1   |
| 9        | 220488       | .5 AMP FUSE                       | 1   |
| 10       | 230105       | FUSE BLOCK 5 X 22 MM              | 1   |
| 11       | 230120       | FUSE...5A.5X22MM                  | 1   |
| 12       | 230135       | FUSE...1A.5X22MM                  | 1   |
| 13       | 400119       | SWITCHER                          | 1   |
| 14       | 400151       | THERMOSTAT 160 F                  | 1   |
| 15       | 515084       | 1/4 DIA. X 3/8L SS SPACER         | 4   |
| 16       | 590032       | #4-40 X 1/4 SS PHP EXT SEMS SCREW | 8   |
| 17       | 730058       | NYLON SHOULDER WASHER             | 4   |
| 18       | 1900312-15-1 | COMPONENT TRAY SUB-ASSEMBLY       | 1   |

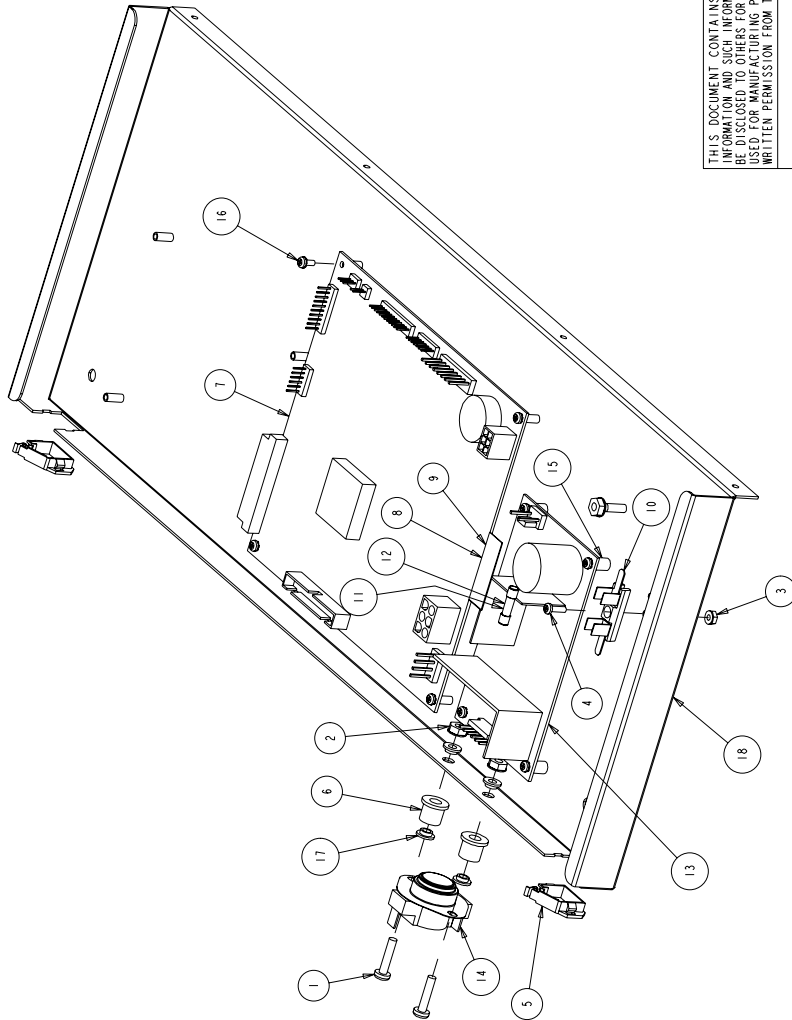

|   |                |                                       |
|---|----------------|---------------------------------------|
| THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSE WITHOUT WRITTEN PERMISSION FROM THERMO ELECTRON |                | MODEL/PART NAME: 370 SERIES INCUBATOR |
|   |                | DWG TITLE: CONTROL PANEL TRAY ASSY    |
| DWN: DALE   | CAD: DCB       | APPD: LDN                             |
| DATE: 3/28/01   | SCALE: 0.500   |                                       |
| MATERIAL: -   |                |                                       |
| PAINT: N/A  |                |                                       |
| TOLERANCE UNLESS OTHERWISE SPECIFIED  |                |                                       |
| ANGLES: .XX±  | DECIMAL: .XXX± | DRAWING NUMBER                        |
|   |                | 370-200-6                             |
|   |                | SIZE                                  |
|   |                | B                                     |


**Thermo**  
Fisher Scientific  
Controlled Environment Equipment  
Box 646, Marietta, OH 45750

1. COMMON TO 3598, 3540, 3541, 3542, 3543

DRAWING NUMBER: 3598-200-7-B

| REV/ECN NO. | DATE    | BY       | CAO | APPD | DESCRIPTION OF REVISION |
|-------------|---------|----------|-----|------|-------------------------|
| 0           | NA      | 06-30-06 | GJG | MSB  | RELEASED FOR PRODUCTION |
| 1           | IN-3759 | 01-15-07 | GJG | CLS  | ADDED COMMON TO NOTE    |

| ITEM | PART NUMBER | PART DESCRIPTION                  | QTY |
|------|-------------|-----------------------------------|-----|
| 1    | 140387      | CONTROL PANEL OVERLAY             | 1   |
| 2    | 1900277     | CONTROL PANEL                     | 1   |
| 3    | 360289      | STERI CYCLE SWITCH (WHITE)        | 1   |
| 4    | 1900346     | CONTROL CIRCUIT BOARD             | 1   |
| 5    | 230180      | CIRCUIT BREAKER SWITCH 12A        | 1   |
| 6    | 360230      | MAGNETIC OUTER DOOR SWITCH        | 1   |
| 7    | 1900355     | SAMPLE PORT BRACKET               | 1   |
| 8    | 23024       | 3/8 SS FLAT WASHER                | 1   |
| 9    | 840065      | 1/4 HOSE X 1/8 FPT BRASS ADAPTER  | 1   |
| 10   | 590027      | 6-32 X 1/4 PHP SEMS SCREW         | 6   |
| 11   | 840035      | 3/16 HOSE X 1/8 MPT BRASS ADAPTER | 1   |
| 12   | 730060      | .416 ID X .628 OD SS WASHER       | 1   |
| 13   | 114011      | 1 1/4 OD X 1/4 ID GROMMET         | 1   |
| 14   | 190294      | FILL PORT RECESS                  | 1   |
| 15   |             |                                   |     |
| 16   |             |                                   |     |
| 17   |             |                                   |     |
| 18   |             |                                   |     |
| 19   |             |                                   |     |
| 20   |             |                                   |     |
| 21   |             |                                   |     |

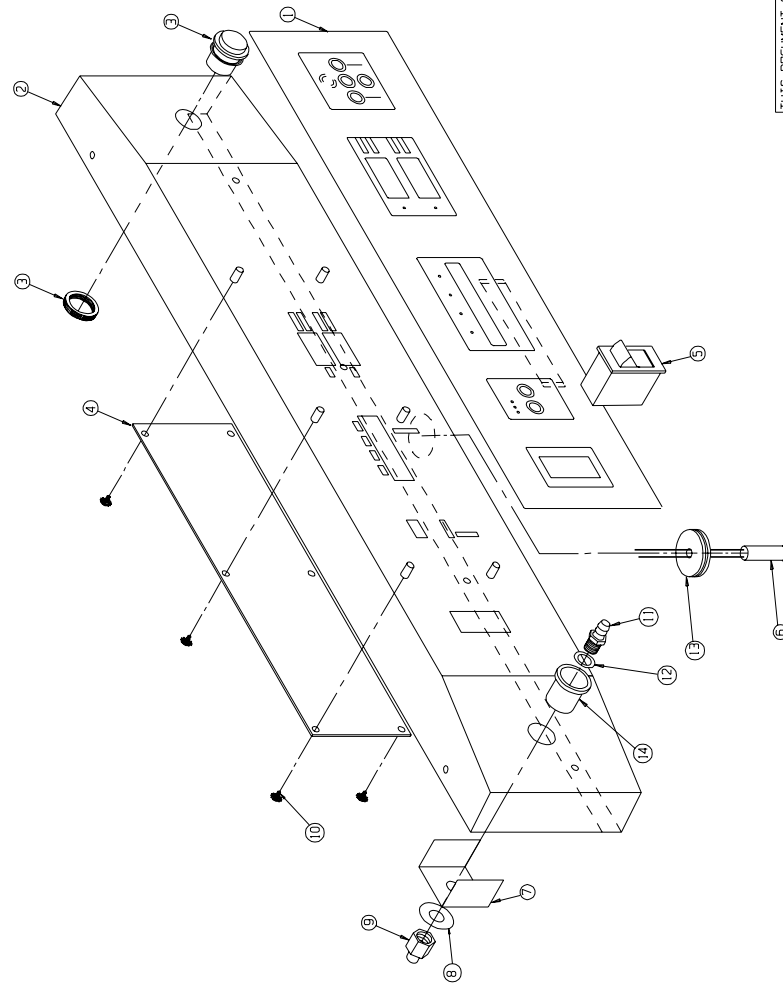

|   |                              |
|---|------------------------------|
| THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSES WITHOUT WRITTEN PERMISSION FROM THERMO ELECTRON. |                              |
| MODEL/PART NAME:  | 3598 SERIES INCUBATOR        |
| DWG TITLE:  | CONTROL PANEL BEZEL ASSEMBLY |
| DMW: GJG  | APPD: GJG                    |
| DATE: 06-30-06  | SCALE: .625                  |
| MATERIAL:   | NA                           |
| PAIN COLOR:   | NA                           |
| TOLERANCE UNLESS OTHERWISE SPECIFIED:   | .XX±                         |
| ANGLES:   | .XXX±                        |
| DRAWING NUMBER  | 3598-200-7                   |
| SIZE  | B                            |



1. COMMON TO: 3840, 3941, 3842 & 3943




DWG. NUMBER: 370-200-8-B

| REV | ECN NO. | DATE     | BY  | CAD APPD | DESCRIPTION OF REVISION                    |
|-----|---------|----------|-----|----------|--|
| 0   | N/A     | 04-24-01 | DCB | LDN      | RELEASED FOR PRODUCTION                    |
| 1   | IN-2915 | 07-06-01 | JGL | MDG      | LDN ADDED 1900118 RING & NUTS TO TC SENSOR |
| 2   | IN-2967 | 09-27-01 | JGL | MDG      | LDN TC SENSOR- ADDED 1900132 HEATER PLATE  |
| 3   | IN-3306 | 06-30-06 | GJG | GJG      | MSB ADDED NOTE # 1                         |
| 4   | IN-3759 | 01-22-07 | GJG | GJG      | ADDED COMMON TO 8000 SERIES                |

| ITEM NO. | PART NO.     | PART DESCRIPTION          | QTY |
|----------|--------------|---------------------------|-----|
| 1        | 22127        | 6-32 x 1.250 SS PHP SCREW | 4   |
| 2        | 23001        | #6-32 ZP LKWASH HEX NUT   | 4   |
| 3        | 244112       | CONVOLUTED TUBE           | 1   |
| 4        | 290168       | HI-TEMP TC SENSOR         | 1   |
| 5        | 1900082      | POLYSULFONE TC MOUNT      | 1   |
| 6        | 1900118      | BELLOWS RESTRAINING RING  | 1   |
| 7        | 1900132      | 370 TC HEATER PLATE       | 1   |
| 8        | 1900327      | TC STOP RING              | 1   |
| 9        | 1900326-31-1 | TC ADAPTER RING           | 1   |

| ITEM NO. | PART NO.     | PART DESCRIPTION         | QTY |
|----------|--------------|--------------------------|-----|
| 1        | 22015        | #8-32 X 3/4 SS PHP SCREW | 4   |
| 2        | 23002        | #8-32 ZP LKWASH HEX NUT  | 4   |
| 3        | 24030        | #8 X 1/2" TEKS SCREW     | 2   |
| 4        | 30088        | 7/8" SNAP BUSHING        | 1   |
| 5        | 103034       | GASKET                   | 1   |
| 6        | 231204       | IR SENSOR                | 1   |
| 7        | 231205       | IR SENSOR MOUNT          | 1   |
| 8        | 244112       | CONVOLUTED TUBE          | 1   |
| 9        | 1900340      | IR STOP 370              | 1   |
| 10       | 1900325-31-1 | IR ADAPTER RING          | 1   |

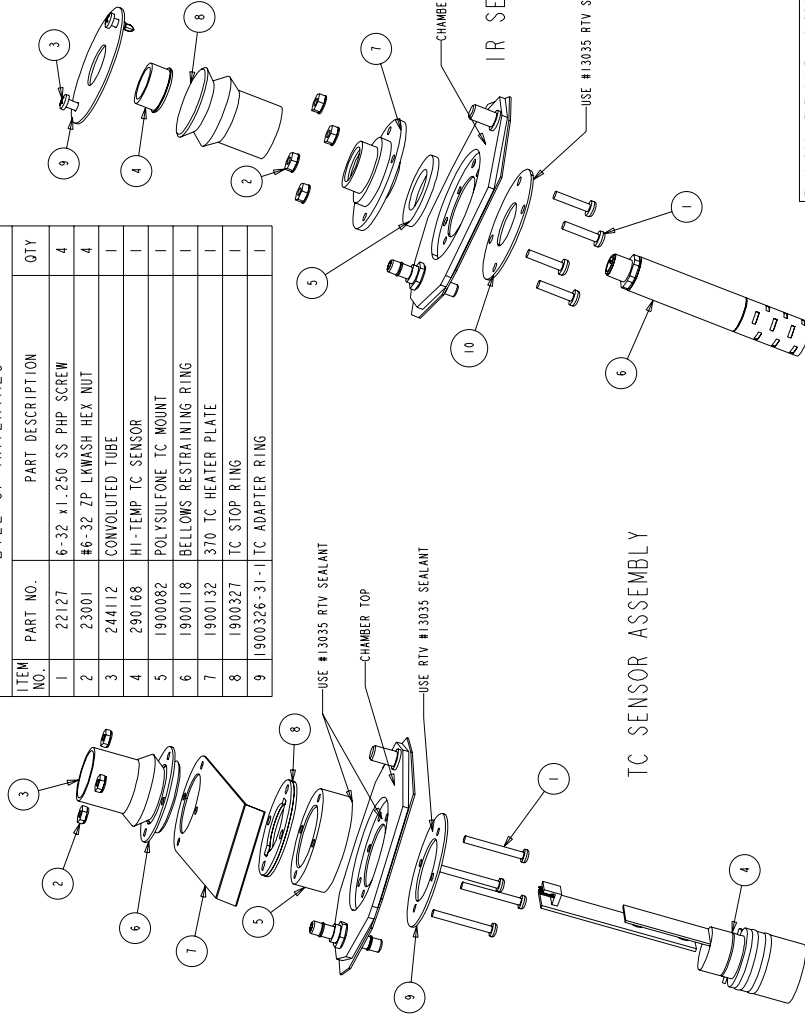

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSE WITHOUT WRITTEN PERMISSION FROM THERMOFISHERSCIENTIFIC


**Thermo**  
ELECTRON CORPORATION  
Controlled Environment Equipment  
Box 647, Norville, OH 43054

MODEL/PART NAME: 370 SERIES INCUBATOR  
DWG TITLE: CO2 SENSORS  
DWG. DATE: CAD: DCB APPD: LDN DATE: 3/27/01 SCALE: 0.500

MATERIAL: -  
PAINT: N/A  
TOLERANCE UNLESS OTHERWISE SPECIFIED ANGLES: .XX± DECIMAL: .XXX±  
DRAWING NUMBER: 370-200-8  
SIZE: B

I. COMONTO 3598, 3540, 3541, 3542, 3543

3598-200-9-0-0 REV. 2  
Page 1 of 2

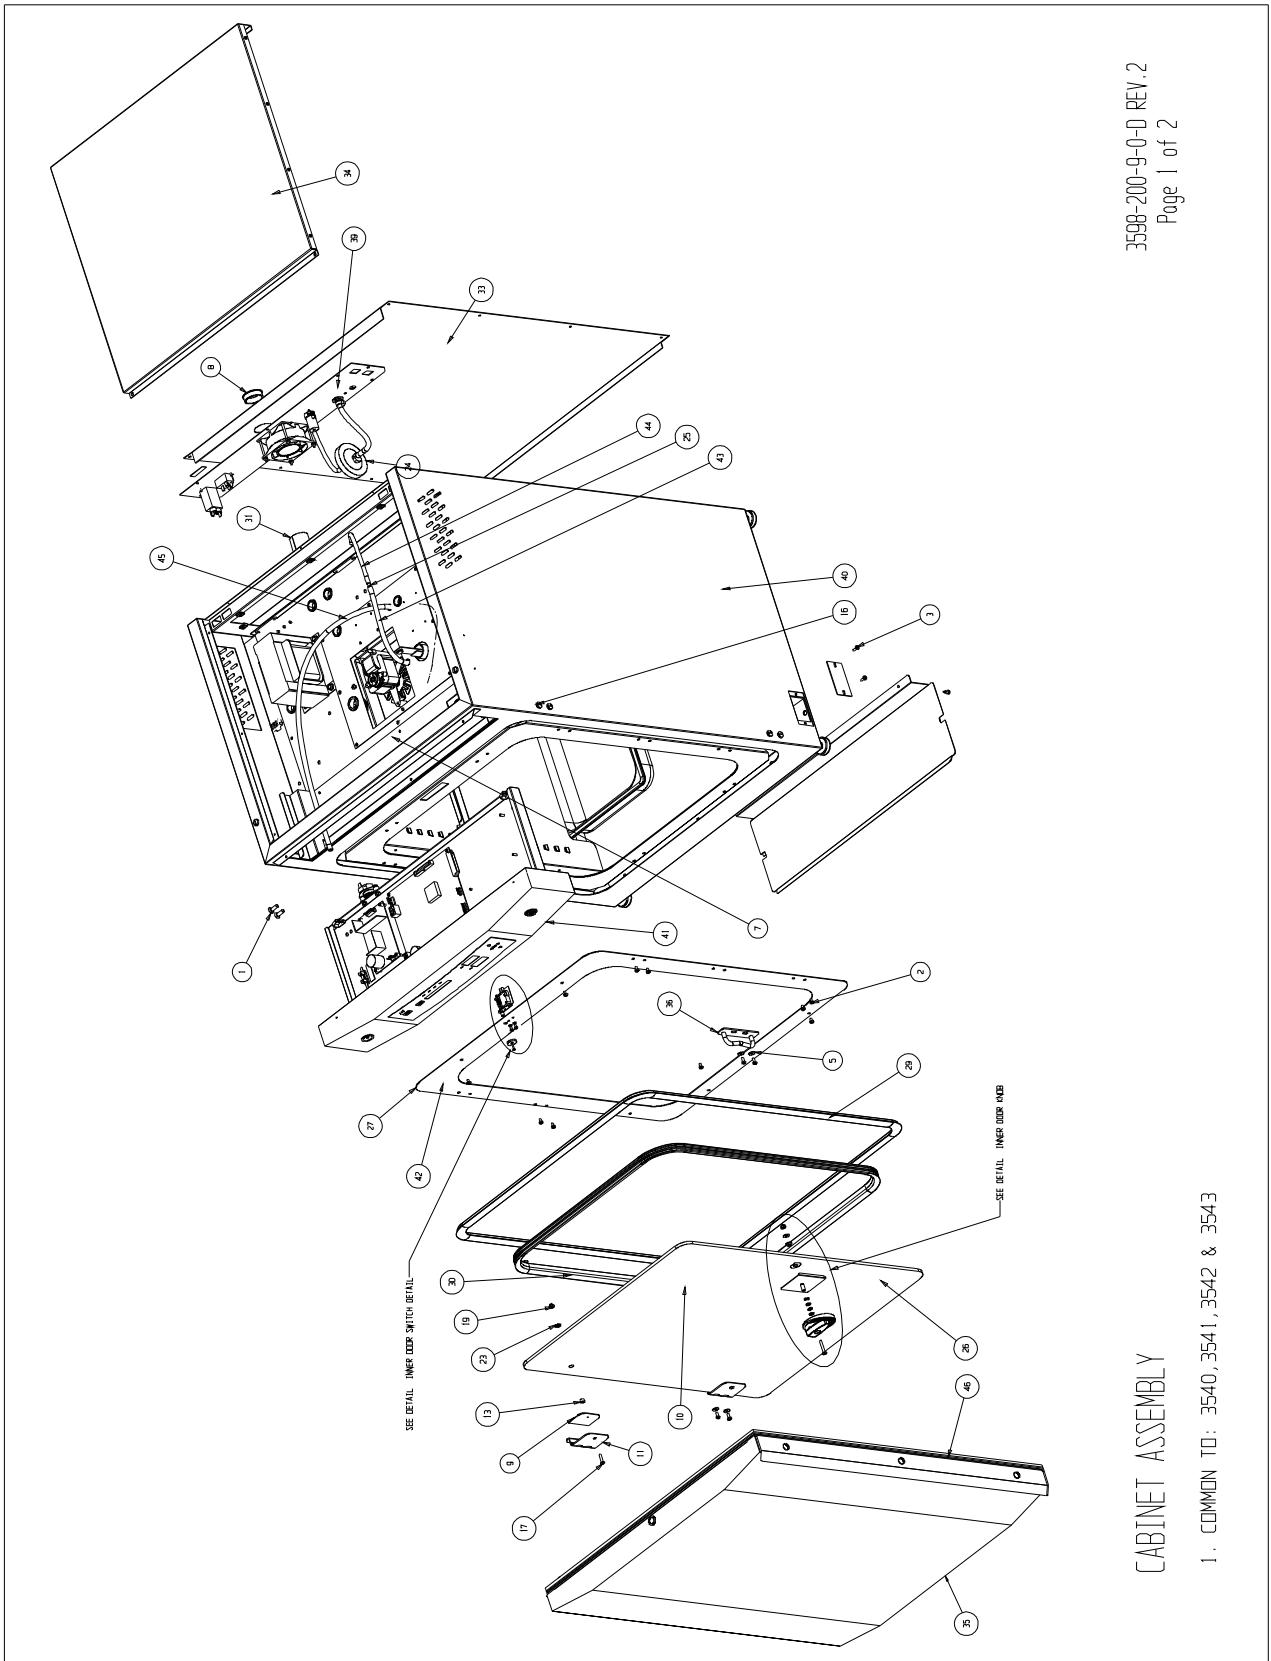

CABINET ASSEMBLY

1. COMMON TO: 3540, 3541, 3542 & 3543

Exploded view diagram of the inner door knob assembly. Callouts 12, 18, 20, 21, and 22 point to various components including the knob, mounting plate, and hardware.

Exploded view diagram of the inner door switch detail. Callouts 4, 6, 14, 15, and 28 point to the switch mechanism, mounting plate, and associated hardware.


DETAIL INNER DOOR KNOB  
SCALE 0.750

DETAIL INNER DOOR SWITCH DETAIL  
SCALE 0.750

| BILL OF MATERIALS |                 |   |     |
|-------------------|-----------------|---|-----|
| ITEM NO.          | PART NO.        | PART DESCRIPTION                        | QTY |
| 1                 | 20058           | #1/4-20 X 3/4 SS FHP UC SCREW           | 4   |
| 2                 | 22051           | #6-32 X 1/4 SS PHP SCREW                | 10  |
| 3                 | 22052           | #6-32 X 3/8 SS PHP SCREW                | 5   |
| 4                 | 22115           | #6-32 X 1/4 SS PHP SCREW                | 2   |
| 5                 | 23021           | #6 SS FLAT WASHER                       | 7   |
| 6                 | 23030           | #6 INTERNAL LOCK WASHER SS              | 2   |
| 7                 | 23051           | #6-32 S.S. WING NUT                     | 4   |
| 8                 | 30077           | 1-1/2" SNAP BUSHING                     | 1   |
| 9                 | 103115          | INNER DOOR HINGE GASKET                 | 2   |
| 10                | 105066          | 20.5 X 26.875 X .23 THK. TEMPER GLASS   | 1   |
| 11                | 116109          | SS HINGE .693 HINGE HEIGHT              | 2   |
| 12                | 120072          | ULTRA HIGH TEMP KNOB DETAIL             | 1   |
| 13                | 125022          | TEFLON SPACER .11/32" O.D.              | 2   |
| 14                | 360239          | INTERLOCK SWITCH                        | 1   |
| 15                | 490026          | 4-40 X 1/2 FHP SS SCREW                 | 1   |
| 16                | 550050          | 1/4-20 X 1/2" NYLON BH SCREW            | 6   |
| 17                | 550054          | #6-32 X 3/4 TRUSS HD PHILLIPS SCREW     | 2   |
| 18                | 550055          | #6-32 X 1-1/8 TRUSS HD PHILLIPS SCREW   | 1   |
| 19                | 610079          | 8-32 SS "FLEXLOC" LOCKING NUT           | 3   |
| 20                | 730056          | .285 ID SS FLAT WASHER                  | 3   |
| 21                | 730057          | WAVE WASHER .288" ID X .407 OD          | 2   |
| 22                | 730073          | TEFLON SHOULDER WASHER                  | 1   |
| 23                | 730086          | 1/2 OD SILICONE SEAL WASHER #B          | 2   |
| 24                | 770001          | DISPOSIBLE HEPTA FILTER 1/4             | 1   |
| 25                | 840026          | 3/16" X 1/4" TUBING REDUCER             | 1   |
| 26                | 1900304         | INNER DOOR ASSEMBLY                     | 1   |
| 27                | 1900318         | INTERIOR FRONT TRIM                     | 1   |
| 28                | 1900338         | 3/4 O.D. INNER DR. SWITCH STRIKE        | 1   |
| 29                | 103102          | HEATBREAK GASKET SILICONE               | 1   |
| 30                | 103108          | INNER DOOR SILICONE GASKET              | 1   |
| 31                | 180115_6        | PORT LINER, TEFLON STRIP 6" LONG        | 1   |
| 32                | 1900182-16-1    | INNER GLASS DOOR KNOB PLATE W/HOLE INT. | 1   |
| 33                | 1900307-31-1    | EXTERIOR BACK                           | 1   |
| 34                | 1900308-16-1    | TOP COVER ASSEMBLY                      | 1   |
| 35                | 3582102-02-1    | EXTERIOR DOOR ASSEMBLY                  | 1   |
| 36                | 1900333-15-1    | INNER DOOR STRIKE ASSEMBLY              | 1   |
| 37                |                 |   |     |
| 38                | 290184          | TEMPERATURE SENSOR                      | 1   |
| 39                | 370-200-5       | 370 BACK PANEL ASSEMBLY                 | 1   |
| 40                | 3701000-01-1    | EXTERIOR WRAP ASSEMBLY                  | 1   |
| 41                | 3578-71-1       | FRONT CONTROL PANEL ASSEMBLY            | 1   |
| 42                | 3705000-01-1    | INNER FACE PLATE ASSY                   | 1   |
| 43                | INJCT. TUBE_1   | CO2 INJECT. TUBE VINYL #72015 6"        | 1   |
| 44                | INJCT. TUBE_2   | CO2 INJECT. TUBE #244020 10"            | 1   |
| 45                | SMP_L. TUBE_370 | SAMPLE TUBE SILICONE #244020 30"        | 1   |
| 46                | 1900290-31-1    | EXTERIOR DOOR HANDLE                    | 1   |


3598-200-9-0-D REV.2  
Page 2 of 2

CABINET ASSEMBLY

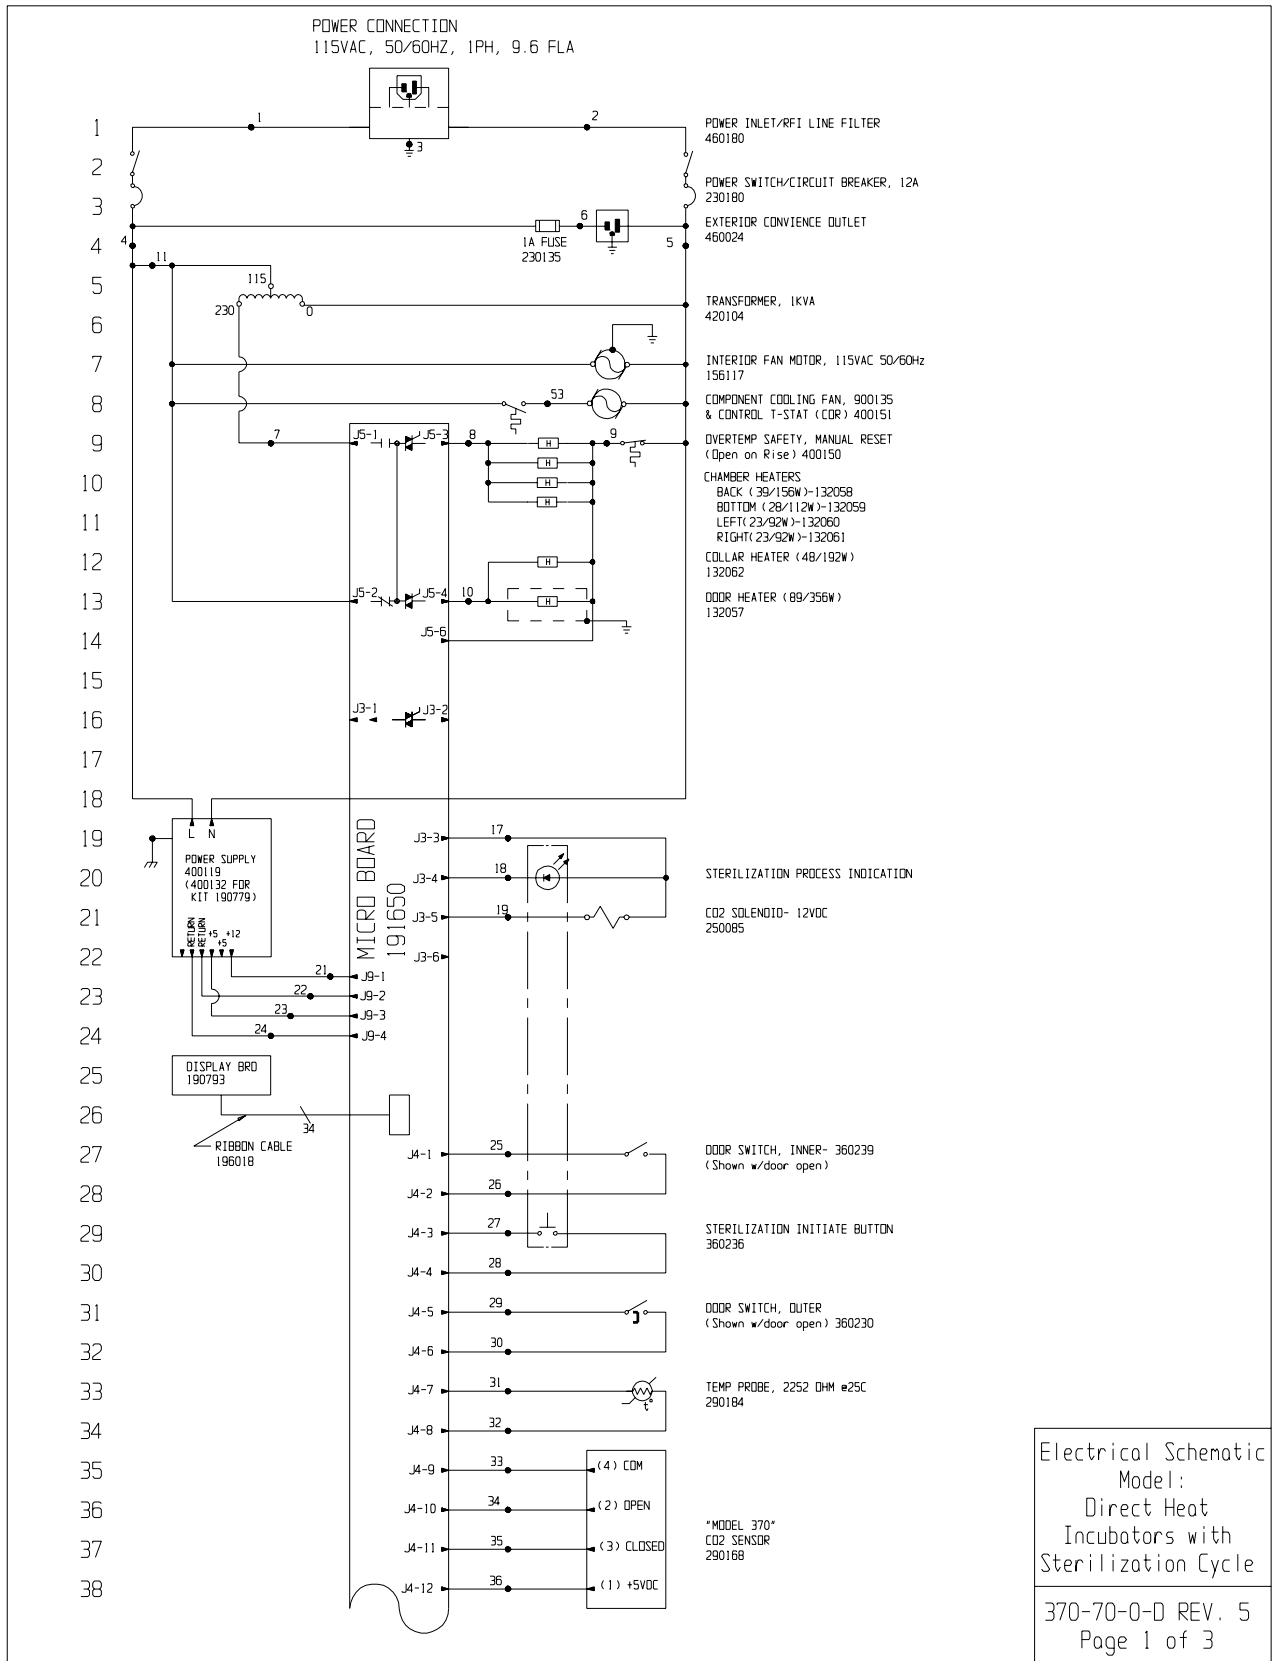

**Section 9**  
Electrical Schematics

39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65  
66  
67  
68  
69  
70  
71  
72  
73  
74  
75  
76

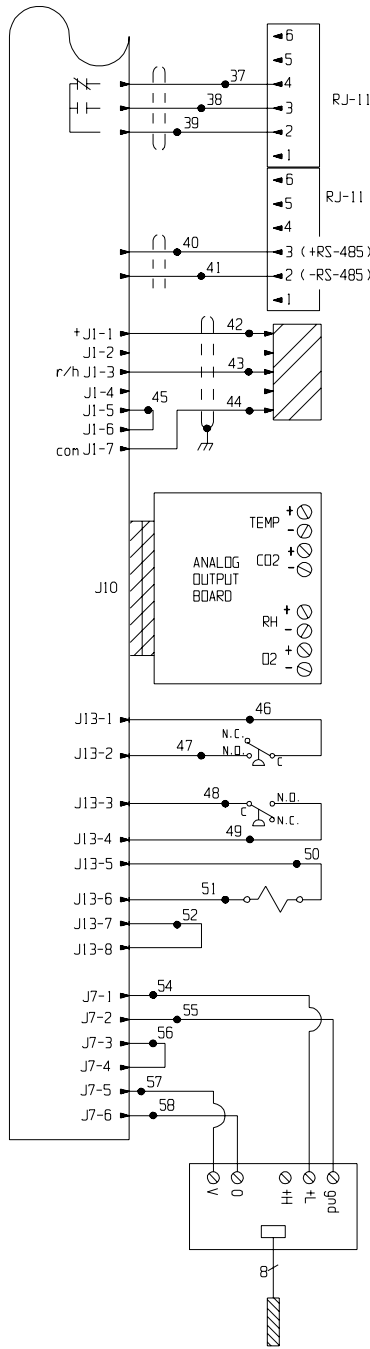

REMOTE ALARM CONNECTIONS  
(shown in alarm state)

"OPTIONAL" RS-485 OUTPUT KIT  
1900085

"OPTIONAL" RH SENSOR KIT  
1900091  
3598  
3599  
3584  
3585

"OPTIONAL" ANALOG OUTPUT KITS  
190512 (4 to 20mA)  
190543 (0 to 5VDC)  
190544 (0 to 1VDC)

"OPTIONAL" GAS GUARD KIT  
1900086 (CO2)

PRESSURE SWITCH #1 (TANK EMPTY)  
360213

PRESSURE SWITCH #2 (TANK EMPTY)  
360213

SOLENOID, 3 WAY- 12VDC  
250121

"MODEL 380"  
IR CO2 SYSTEM  
231204

Electrical Schematic  
Model:  
Direct Heat  
Incubators with  
Sterilization Cycle

370-70-0-D REV. 5  
Page 2 of 3

77  
78  
79  
80  
81  
82  
83  
84  
85  
86  
87  
88  
89  
90  
91  
92  
93  
94  
95  
96  
97  
98  
99

| WIRE REFERENCE CHART |     |         |     |      |        |     |      |        |
|----------------------|-----|---------|-----|------|--------|-----|------|--------|
| NO.                  | GA. | COLOR   | NO. | GA.  | COLOR  | NO. | GA.  | COLOR  |
| 1                    | 16  | BROWN   | 21  | 18   | RED    | 42  | 22/3 | BLACK  |
| 2                    | 16  | BLUE    | 22  | 18   | GREEN  | 43  | 22/3 | RED    |
| 3                    | 16  | GRN/YEL | 23  | 18   | ORANGE | 44  | 22/3 | GREEN  |
| 4                    | 16  | BLACK   | 24  | 18   | GREEN  | 45  | 22   | BLACK  |
| 5                    | 16  | WHITE   | 25  | 22   | BLUE   | 46  | 20   | RED    |
| 6                    | 18  | BLACK   | 26  | 22   | BLUE   | 47  | 20   | RED    |
| 7                    | 16  | YELLOW  | 27  | 22   | BROWN  | 48  | 20   | BLUE   |
| 8                    | 18  | ORANGE  | 28  | 22   | BROWN  | 49  | 20   | BLUE   |
| 9                    | 18  | RED     | 29  | 22   | YELLOW | 50  | 20   | ORANGE |
| 10                   | 18  | BLUE    | 30  | 22   | YELLOW | 51  | 20   | ORANGE |
| 11                   | 18  | RED     | 31  | 22   | RED    | 52  | 20   | BLACK  |
| 12                   | --  | ----    | 32  | 22   | RED    | 53  | 18   | BROWN  |
| 13                   | --  | ----    | 33  | 22   | GREEN  | 54  | 24/4 | BLACK  |
| 14                   | --  | ----    | 34  | 22   | GRAY   | 55  | 24/4 | WHITE  |
| 15                   | --  | ----    | 35  | 22   | PURPLE | 56  | 24   | BLACK  |
| 16                   | --  | ----    | 36  | 22   | ORANGE | 57  | 24/4 | RED    |
| 17                   | 18  | ORANGE  | 37  | 22/3 | BLACK  | 58  | 24/4 | GREEN  |
| 18                   | 18  | BLACK   | 38  | 22/3 | RED    | 59  |      |        |
| 19                   | 18  | YELLOW  | 39  | 22/3 | WHITE  | 60  |      |        |
| 20                   | --  | ----    | 40  | 22/2 | RED    |     |      |        |
|                      |     |         | 41  | 22/2 | BLACK  |     |      |        |

| MODEL | DESCRIPTION                               |
|-------|---|
| 370   | STERI CYCLE 1/2 CO2 INCUBATOR             |
| 380   | STERI CYCLE 1/4 CO2 INCUBATOR             |
| 3598  | STERI CYCLE 1/2 CO2 INCUBATOR             |
| 3599  | STERI CYCLE 1/4 CO2 INCUBATOR             |
| 3584  | STERI CYCLE 1/2 CO2 INCUBATOR, RH DISPLAY |
| 3585  | STERI CYCLE 1/4 CO2 INCUBATOR, RH DISPLAY |
| 3540  | STERI CYCLE 1/2 CO2 INCUBATOR, 115 VOLT   |
| 3542  | STERI CYCLE 1/4 CO2 INCUBATOR, 115 VOLT   |

|     |         |          |        |        |      |  |
|-----|---------|----------|--------|--------|------|--|
| 5   | IN-3759 | 01-15-07 | G.J.G. | G.J.G. | CCS  | ADDED MODEL NUMBERS                          |
| 4   | IN-3306 | 06-15-06 | G.J.G. | G.J.G. | MSB  | ADDED MODEL NUMBERS                          |
| 3   | IN-3124 | 08-04-03 | JNL    | KDG    | LDN  | CHANGED 290137 TEMP. PROBE TO 290184         |
| 2   | IN-2970 | 09-04-01 | GLM    | KDG    | LDN  | CHG. HARNESS FOR MICRO TO SENSE VOLTAGE LOSS |
| 1   | IN-2915 | 04-03-01 | GLM    | KDG    | DNF  | CHANGED 130625 COOLING FAN TO 900135         |
| 0   | N/A     | 1-23-01  | GM     | GM     | DNF  | RELEASED PRODUCTION                          |
| REV | ECN NO. | DATE     | BY     | CAO    | APPO | DESCRIPTION OF REVISION                      |

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSES WITHOUT WRITTEN PERMISSION FROM THERMO ELECTRON.

MODEL/PART NAME: HEAT STERILIZATION INCUBATOR (See Above)  
 DWG TITLE: ELECTRICAL SCHEMATIC  
 DWG: 4M CAD: 4M APPD: DNF DATE: 9-12-00 SCALE: NONE



**ATTENTION**  
OBSERVE PRECAUTIONS  
**ELECTROSTATIC SENSITIVE DEVICES**




MATERIAL:  
 PAINT COLOR:  
 TOLERANCE UNLESS OTHERWISE SPECIFIED: .XX±  
 ANGLES: DECIMAL: .XX±

DRAWING NUMBER  
370-70-0

Electrical Schematic  
 Model:  
 Direct Heat  
 Incubators with  
 Sterilization Cycle


370-70-0-D REV. 5  
 Page 3 of 3



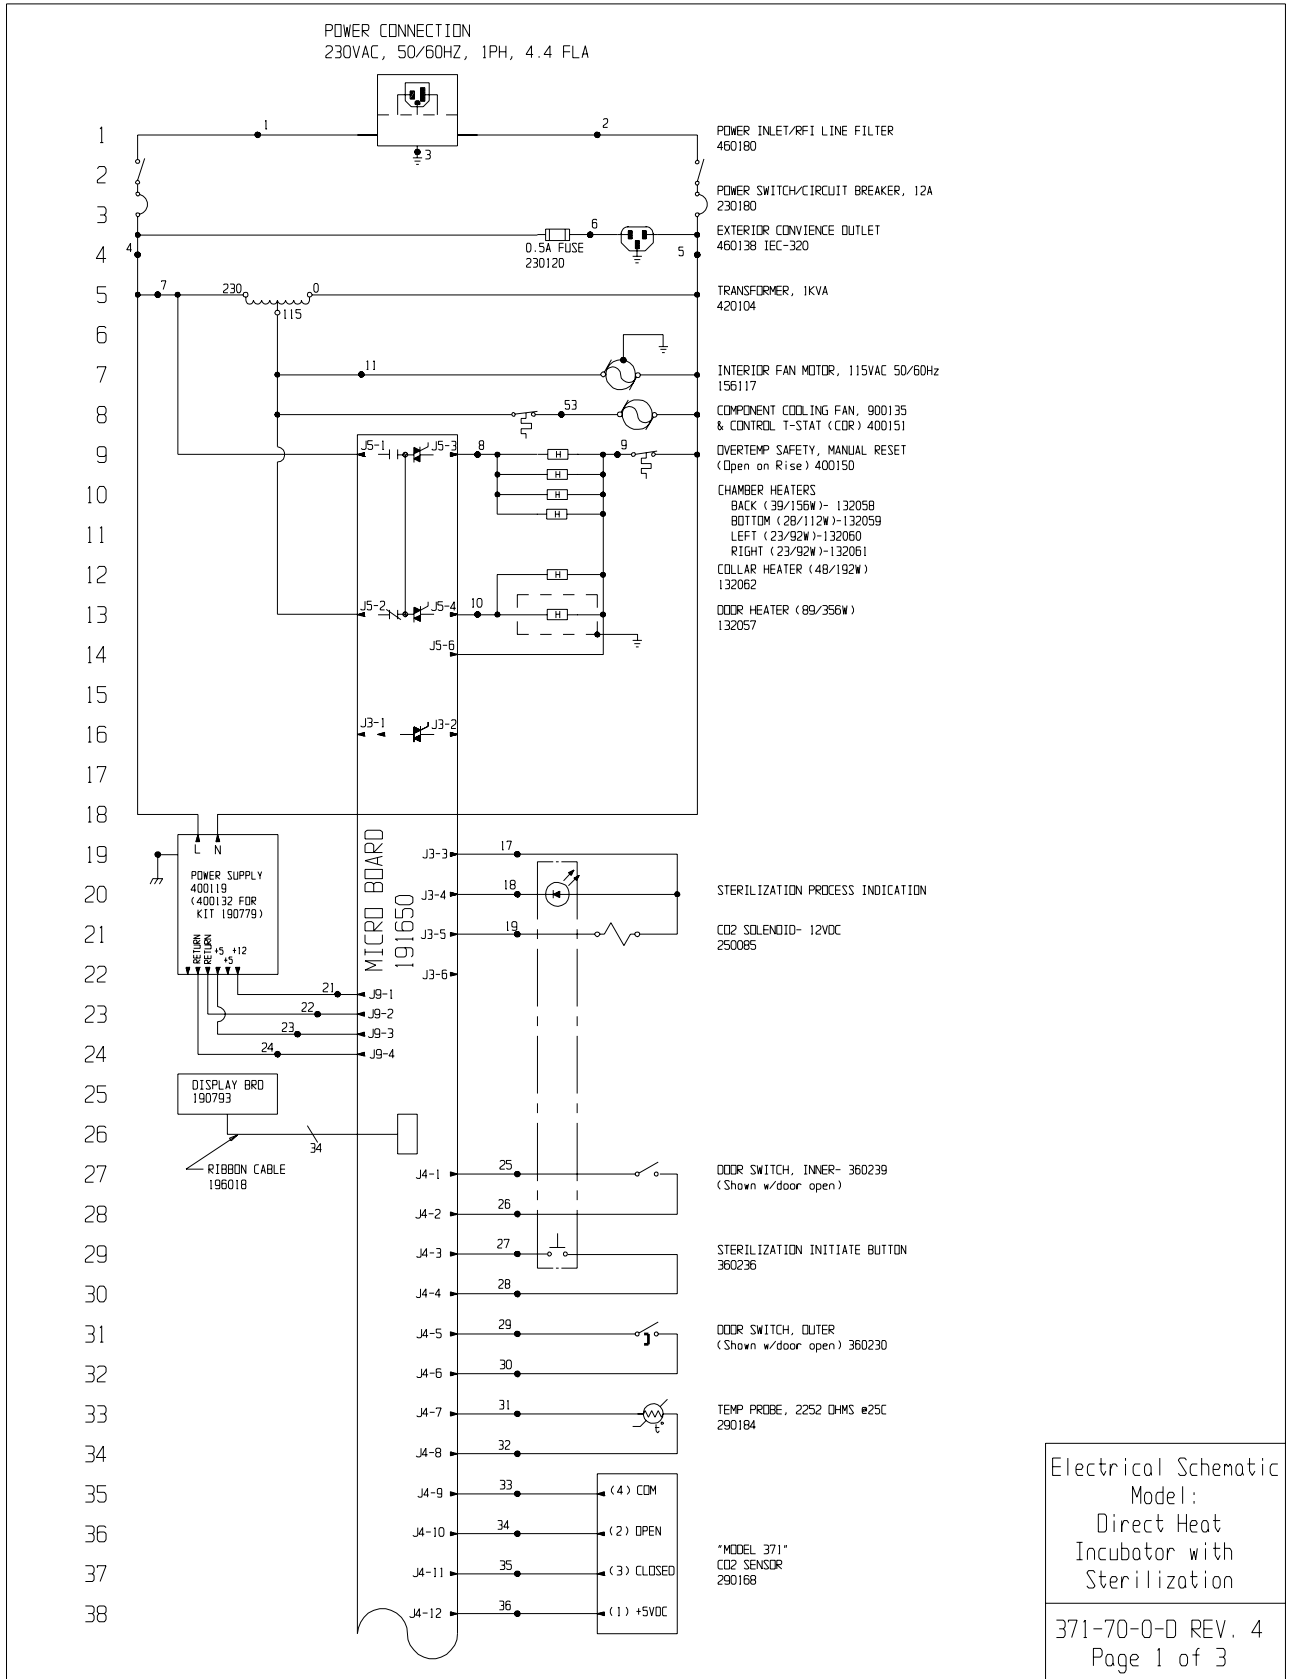



**Section 9**  
Electrical Schematics

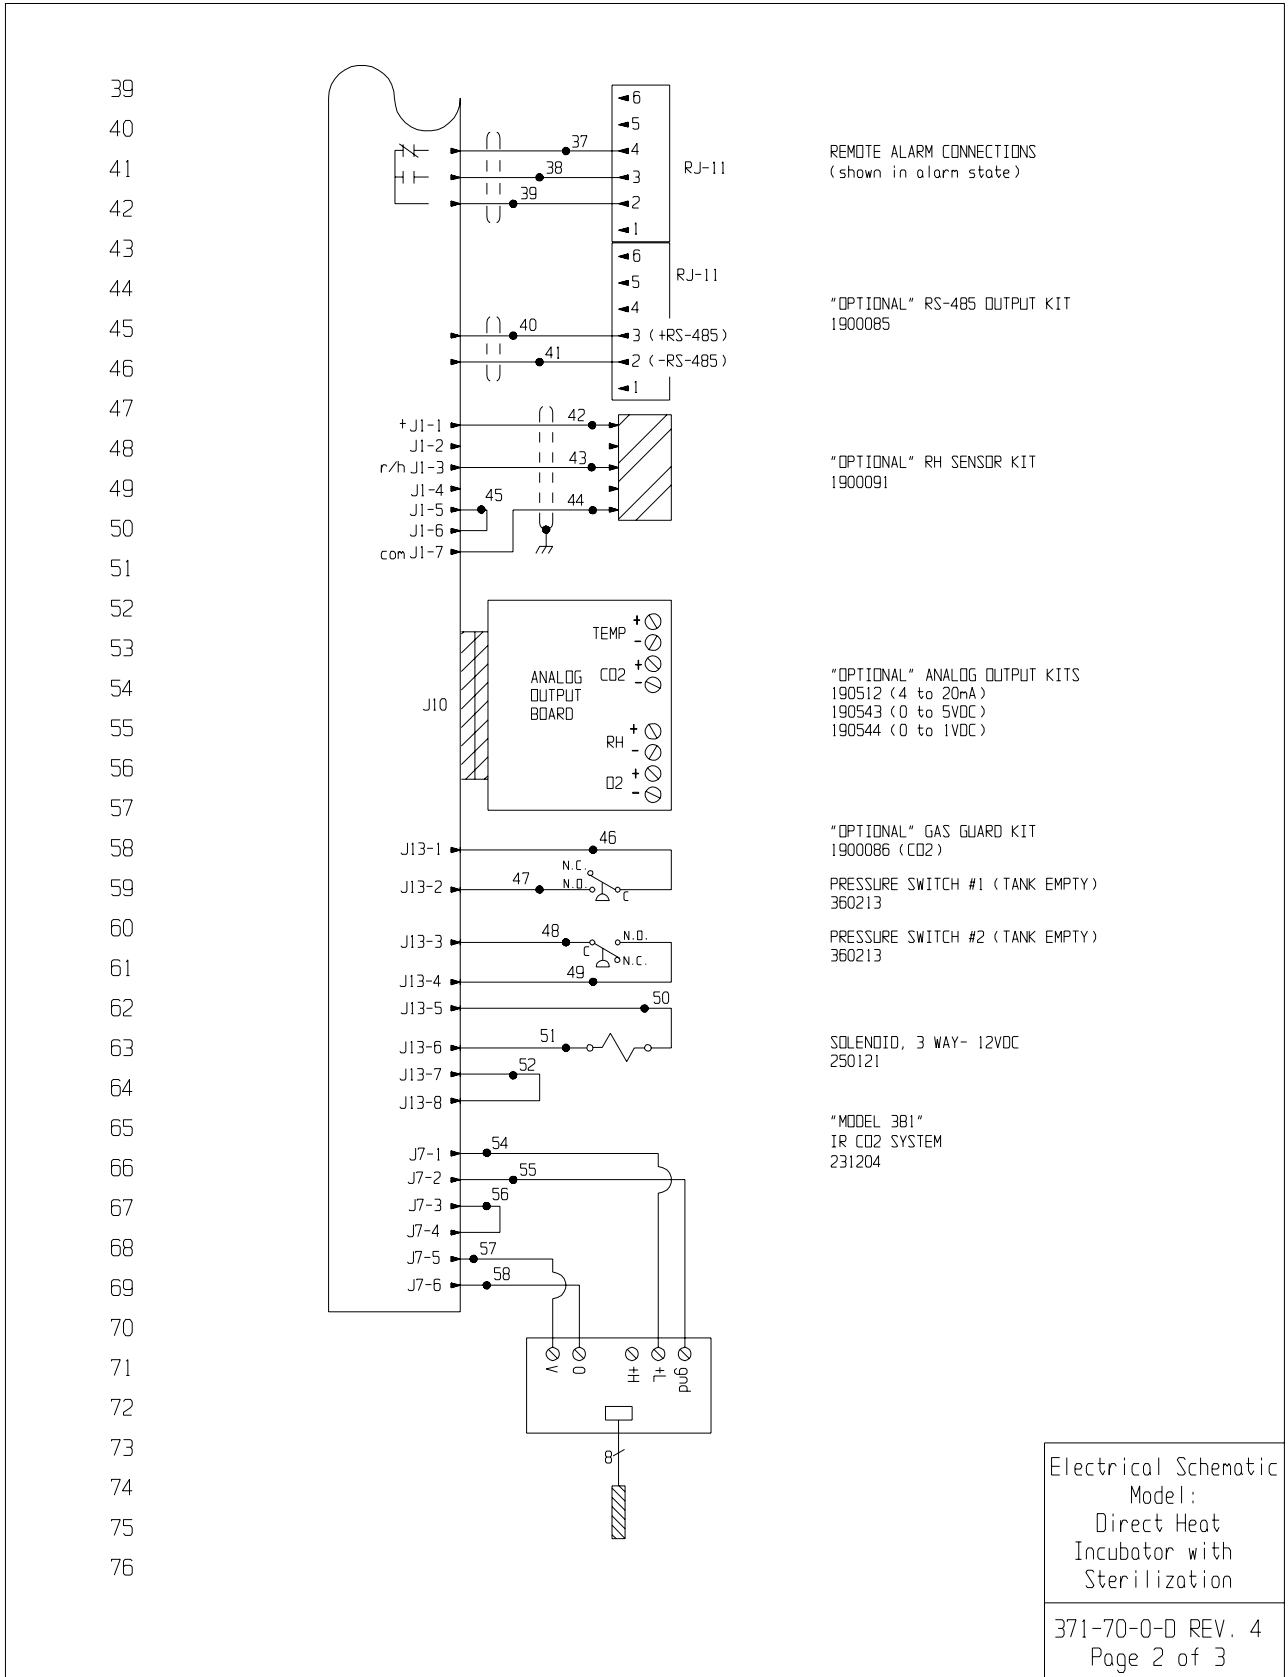

77  
78  
79  
80  
81  
82  
83  
84  
85  
86  
87  
88  
89  
90  
91  
92  
93  
94  
95  
96  
97  
98  
99  
100  
101  
102  
103  
104  
105  
106  
107

| WIRE REFERENCE CHART |     |         |     |      |        |     |      |        |
|----------------------|-----|---------|-----|------|--------|-----|------|--------|
| NO.                  | GA. | COLOR   | NO. | GA.  | COLOR  | NO. | GA.  | COLOR  |
| 1                    | 16  | BROWN   | 21  | 18   | RED    | 42  | 22/3 | BLACK  |
| 2                    | 16  | BLUE    | 22  | 18   | GREEN  | 43  | 22/3 | RED    |
| 3                    | 16  | GRN/YEL | 23  | 18   | ORANGE | 44  | 22/3 | GREEN  |
| 4                    | 16  | BLACK   | 24  | 18   | GREEN  | 45  | 22   | BLACK  |
| 5                    | 16  | WHITE   | 25  | 22   | BLUE   | 46  | 20   | RED    |
| 6                    | 18  | BLACK   | 26  | 22   | BLUE   | 47  | 20   | RED    |
| 7                    | 16  | YELLOW  | 27  | 22   | BROWN  | 48  | 20   | BLUE   |
| 8                    | 18  | ORANGE  | 28  | 22   | BROWN  | 49  | 20   | BLUE   |
| 9                    | 18  | RED     | 29  | 22   | YELLOW | 50  | 20   | ORANGE |
| 10                   | 18  | BLUE    | 30  | 22   | YELLOW | 51  | 20   | ORANGE |
| 11                   | 18  | RED     | 31  | 22   | RED    | 52  | 20   | BLACK  |
| 12                   | --  | ----    | 32  | 22   | RED    | 53  | 18   | BROWN  |
| 13                   | --  | ----    | 33  | 22   | GREEN  | 54  | 24/4 | BLACK  |
| 14                   | --  | ----    | 34  | 22   | GRAY   | 55  | 24/4 | WHITE  |
| 15                   | --  | ----    | 35  | 22   | PURPLE | 56  | 24   | BLACK  |
| 16                   | --  | ----    | 36  | 22   | ORANGE | 57  | 24/4 | RED    |
| 17                   | 18  | ORANGE  | 37  | 22/3 | BLACK  | 58  | 24/4 | GREEN  |
| 18                   | 18  | BLACK   | 38  | 22/3 | RED    | 59  |      |        |
| 19                   | 18  | YELLOW  | 39  | 22/3 | WHITE  | 60  |      |        |
| 20                   | --  | ----    | 40  | 22/2 | RED    |     |      |        |
|                      |     |         | 41  | 22/2 | BLACK  |     |      |        |

| MODEL | DESCRIPTION                    |
|-------|--------------------------------|
| 3541  | STERI-CYCLE TC CO2 INC. - 230V |
| 3543  | STERI-CYCLE IR CO2 INC. - 230V |

|     |         |          |     |      |                         |  |
|-----|---------|----------|-----|------|-------------------------|--|
| 4   | IN-3759 | 01-22-07 | GJG | GJG  | CCS                     | ADDED DH 8000 SERIES MODELS                  |
| 3   | IN-3124 | 08-04-03 | JNL | KDC  | LON                     | CHANGED 290137 TEMP. PROBE TO 290184         |
| 2   | IN-2970 | 09-04-01 | GLM | KDC  | LON                     | CHG. HARNESS FOR MICRO TO SENSE VOLTAGE LOSS |
| 1   | IN-2915 | 04-02-01 | GLM | KDC  | DNF                     | CHG. 130625 FAN TO 900135 & REV. FLA         |
| 0   | N/A     | 1-23-01  | GJM | GJM  | DNF                     | RELEASED FOR PRODUCTION                      |
| REV | NO.     | DATE     | BY  | APPD | DESCRIPTION OF REVISION |  |

Electrical Schematic  
Model:  
Direct Heat  
Incubator with  
Sterilization

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND SUCH INFORMATION IS NOT TO BE DISCLOSED TO OTHERS FOR ANY PURPOSE NOR USED FOR MANUFACTURING PURPOSES WITHOUT WRITTEN PERMISSION FROM THERMO ELECTRON

MODEL/PART NAME: 371 & 381 HEAT STERILIZATION INCUBATOR  
DWG TITLE: ELECTRICAL SCHEMATIC  
DWN: GJM CAD: GJM APPD: DNF DATE: 9-12-00 SCALE: NONE



**ATTENTION**  
OBSERVE PRECAUTIONS  
ELECTROSTATIC  
SENSITIVE DEVICES



MATERIAL:  
PAINT COLOR:  
TOLERANCE UNLESS OTHERWISE SPECIFIED: XX±  
ANGLES: DECIMAL: XXX±

DRAWING NUMBER  
371-70-0

371-70-0-0 REV. 4  
Page 3 of 3



## **THERMO FISHER SCIENTIFIC STANDARD PRODUCT WARRANTY**

The Warranty Period starts two weeks from the date your equipment is shipped from our facility. This allows for shipping time so the warranty will go into effect at approximately the same time your equipment is delivered. The warranty protection extends to any subsequent owner during the first year warranty period.

During the first year, component parts proven to be non-conforming in materials or workmanship will be repaired or replaced at Thermo's expense, labor included. Installation and calibration are not covered by this warranty agreement. The Technical Services Department must be contacted for warranty determination and direction prior to performance of any repairs. Expendable items, glass, filters and gaskets are excluded from this warranty.

Replacement or repair of components parts or equipment under this warranty shall not extend the warranty to either the equipment or to the component part beyond the original warranty period. The Technical Services Department must give prior approval for return of any components or equipment. At Thermo's option, all non-conforming parts must be returned to Thermo Electron Corporation postage paid and replacement parts are shipped FOB destination.

**THIS WARRANTY IS EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES, WHETHER WRITTEN, ORAL OR IMPLIED. NO WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE SHALL APPLY.** Thermo shall not be liable for any indirect or consequential damages including, without limitation, damages relating to lost profits or loss of products.

Your local Thermo Sales Office is ready to help with comprehensive site preparation information before your equipment arrives. Printed instruction manuals carefully detail equipment installation, operation and preventive maintenance.

If equipment service is required, please call your Technical Services Department at 1-800-438-4851 (USA and Canada) or 1-740-373-4763. We're ready to answer your questions on equipment warranty, operation, maintenance, service and special application. Outside the USA, contact your local distributor for warranty information.



Rev. 4 4/09

## **THERMO FISHER SCIENTIFIC INTERNATIONAL DEALER WARRANTY**

The Warranty Period starts two months from the date your equipment is shipped from our facility. This allows for shipping time so the warranty will go into effect at approximately the same time your equipment is delivered. The warranty protection extends to any subsequent owner during the first year warranty period. Dealers who stock our equipment are allowed an additional six months for delivery and installation, provided the warranty card is completed and returned to the Technical Services Department.

During the first year, component parts proven to be non-conforming in materials or workmanship will be repaired or replaced at Thermo's expense, labor excluded. Installation and calibration are not covered by this warranty agreement. The Technical Services Department must be contacted for warranty determination and direction prior to performance of any repairs. Expendable items, glass, filters, reagents, tubing, and gaskets are excluded from this warranty.

Replacement or repair of components parts or equipment under this warranty shall not extend the warranty to either the equipment or to the component part beyond the original warranty period. The Technical Services Department must give prior approval for return of any components or equipment. At Thermo's option, all non-conforming parts must be returned to Thermo postage paid and replacement parts are shipped FOB destination.

**THIS WARRANTY IS EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES, WHETHER WRITTEN, ORAL OR IMPLIED. NO WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE SHALL APPLY.** Thermo shall not be liable for any indirect or consequential damages including, without limitation, damages relating to lost profits or loss of products.

Your local Thermo Sales Office is ready to help with comprehensive site preparation information before your equipment arrives. Printed instruction manuals carefully detail equipment installation, operation and preventive maintenance.

Contact your local distributor for warranty information. We're ready to answer your questions on equipment warranty, operation, maintenance, service and special application.



# Declaration of Conformity

**Manufacturer's Name:** Thermo Fisher Scientific (Asheville) LLC  
**Manufacturer's Address:** 401 Millcreek Road  
Marietta, Ohio 45750  
U.S.A.  
**Product Description:** Thermo Laboratory Incubator  
**Product Designations:** 3540  
**Year of Initial Marking (CE):** 2007  
**Affected Serial Numbers:** Release 1  
(Release Level [REL#] shown on serial tag)

This product conforms to the following European Union Directive(s):

**EMC:** 89/336/EEC  
**LVD:** 73/23/EEC

This product conforms to the following Harmonized, International and National Standards:

| <b>EMC:</b>               | <b>LVD:</b>          |
|---------------------------|----------------------|
| EN 61326-1:1997 (Class A) | EN 61010-1:1993      |
| EN 50081-1                | Amendments 1 and 2   |
| EN 50082-1                | CSA C22.2 No. 1010.1 |
| EN 50011-1:97             | UL 61010-1           |
|                           | UL 61010-2-010       |

  
Richard L. Miller, CQE  
Regulatory Compliance Manager

**ThermoFisher**  
S C I E N T I F I C

25 January 2007

# Declaration of Conformity

**Manufacturer's Name:** Thermo Fisher Scientific (Asheville) LLC  
**Manufacturer's Address:** 401 Millcreek Road  
Marietta, Ohio 45750  
U.S.A.  
**Product Description:** Thermo Laboratory Incubator  
**Product Designations:** 3541  
**Year of Initial Marking (CE):** 2007  
**Affected Serial Numbers:** Release 1  
(Release Level [REL#] shown on serial tag)

This product conforms to the following European Union Directive(s):

**EMC:** 89/336/EEC  
**LVD:** 73/23/EEC

This product conforms to the following Harmonized, International and National Standards:

| <b>EMC:</b>               | <b>LVD:</b>          |
|---------------------------|----------------------|
| EN 61326-1:1997 (Class A) | EN 61010-1:1993      |
| EN 50081-1                | Amendments 1 and 2   |
| EN 50082-1                | CSA C22.2 No. 1010.1 |
| EN 50011-1:97             | UL 61010-1           |
|                           | UL 61010-2-010       |

  
Richard L. Miller, CQE  
Regulatory Compliance Manager

**ThermoFisher**  
S C I E N T I F I C

25 January 2007

# Declaration of Conformity


**Manufacturer's Name:** Thermo Fisher Scientific (Asheville) LLC  
**Manufacturer's Address:** 401 Millcreek Road  
Marietta, Ohio 45750  
U.S.A.  
**Product Description:** Thermo Laboratory Incubator  
**Product Designations:** 3542  
**Year of Initial Marking (CE):** 2007  
**Affected Serial Numbers:** Release 1  
(Release Level [REL#] shown on serial tag)

This product conforms to the following European Union Directive(s):

**EMC:** 89/336/EEC  
**LVD:** 73/23/EEC

This product conforms to the following Harmonized, International and National Standards:

| <b>EMC:</b>               | <b>LVD:</b>          |
|---------------------------|----------------------|
| EN 61326-1:1997 (Class A) | EN 61010-1:1993      |
| EN 50081-1                | Amendments 1 and 2   |
| EN 50082-1                | CSA C22.2 No. 1010.1 |
| EN 50011-1:97             | UL 61010-1           |
|                           | UL 61010-2-010       |

  
Richard L. Miller, CQE  
Regulatory Compliance Manager

**ThermoFisher**  
S C I E N T I F I C

25 January 2007

# Declaration of Conformity


**Manufacturer's Name:** Thermo Fisher Scientific (Asheville) LLC  
**Manufacturer's Address:** 401 Millcreek Road  
Marietta, Ohio 45750  
U.S.A.  
**Product Description:** Thermo Laboratory Incubator  
**Product Designations:** 3543  
**Year of Initial Marking (CE):** 2007  
**Affected Serial Numbers:** Release 1  
(Release Level [REL#] shown on serial tag)

This product conforms to the following European Union Directive(s):

**EMC:** 89/336/EEC  
**LVD:** 73/23/EEC

This product conforms to the following Harmonized, International and National Standards:

| <b>EMC:</b>               | <b>LVD:</b>          |
|---------------------------|----------------------|
| EN 61326-1:1997 (Class A) | EN 61010-1:1993      |
| EN 50081-1                | Amendments 1 and 2   |
| EN 50082-1                | CSA C22.2 No. 1010.1 |
| EN 50011-1:97             | UL 61010-1           |
|                           | UL 61010-2-010       |

  
Richard L. Miller, CQE  
Regulatory Compliance Manager

**ThermoFisher**  
S C I E N T I F I C

25 January 2007



Thermo Scientific  
Controlled Environment Equipment  
401 Millcreek Road  
Marietta, Ohio 45750  
United States

[www.thermofisher.com](http://www.thermofisher.com)